

1



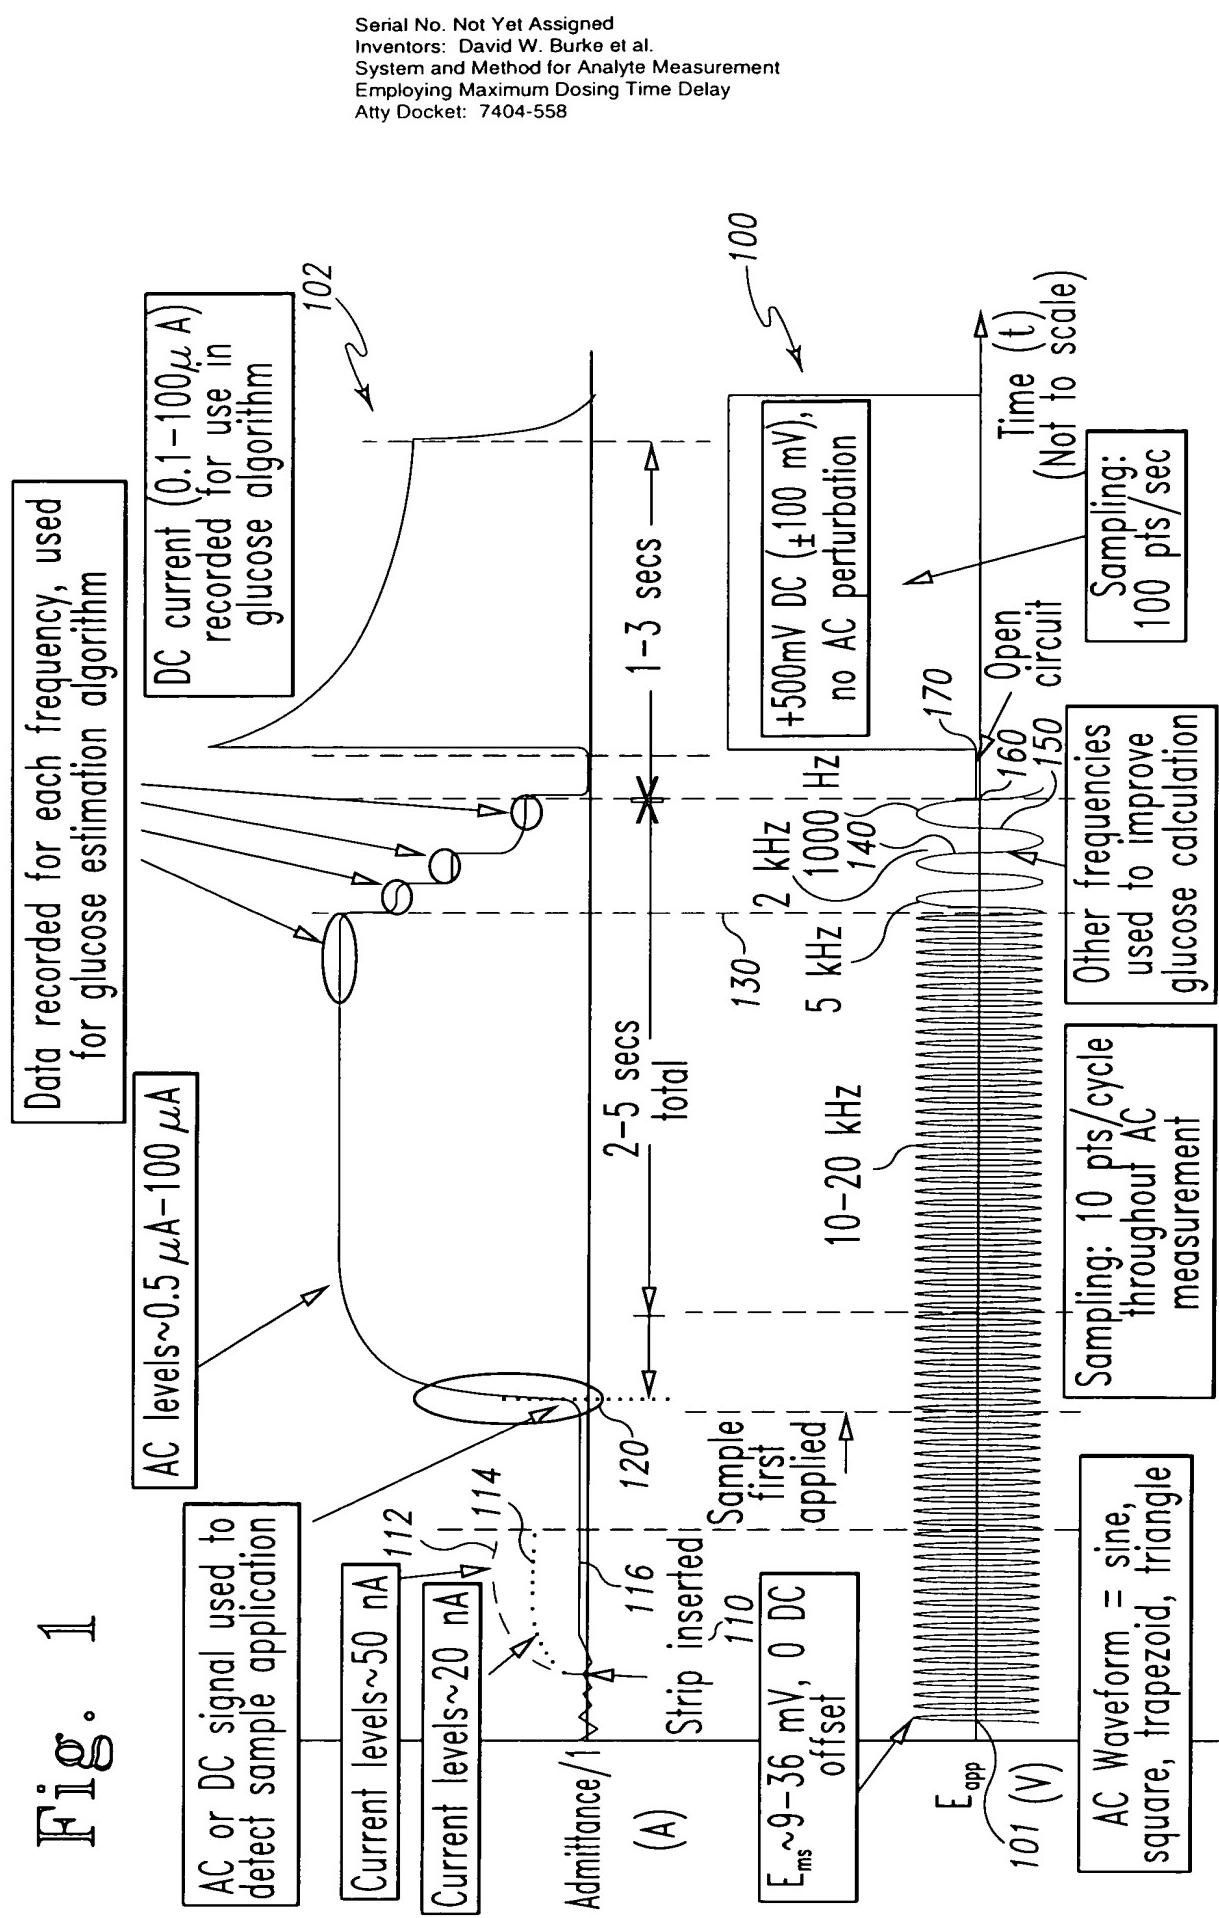


Fig. 2

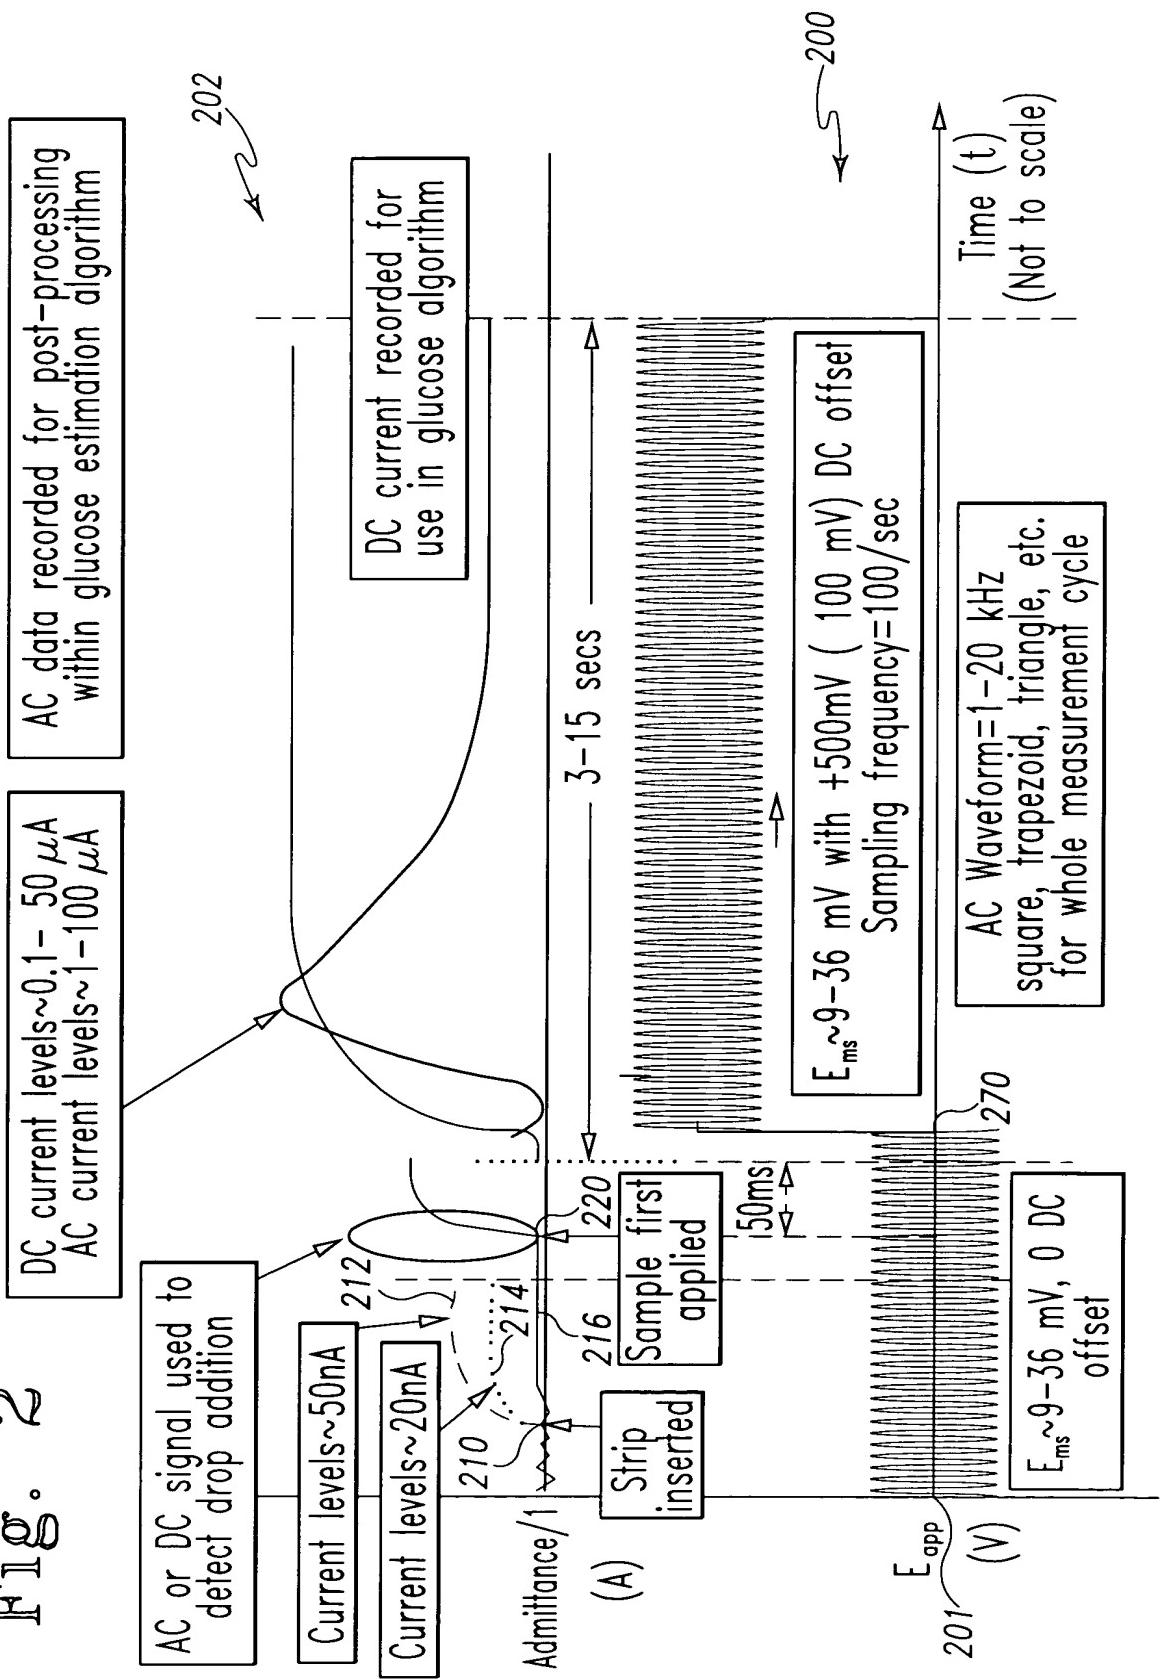

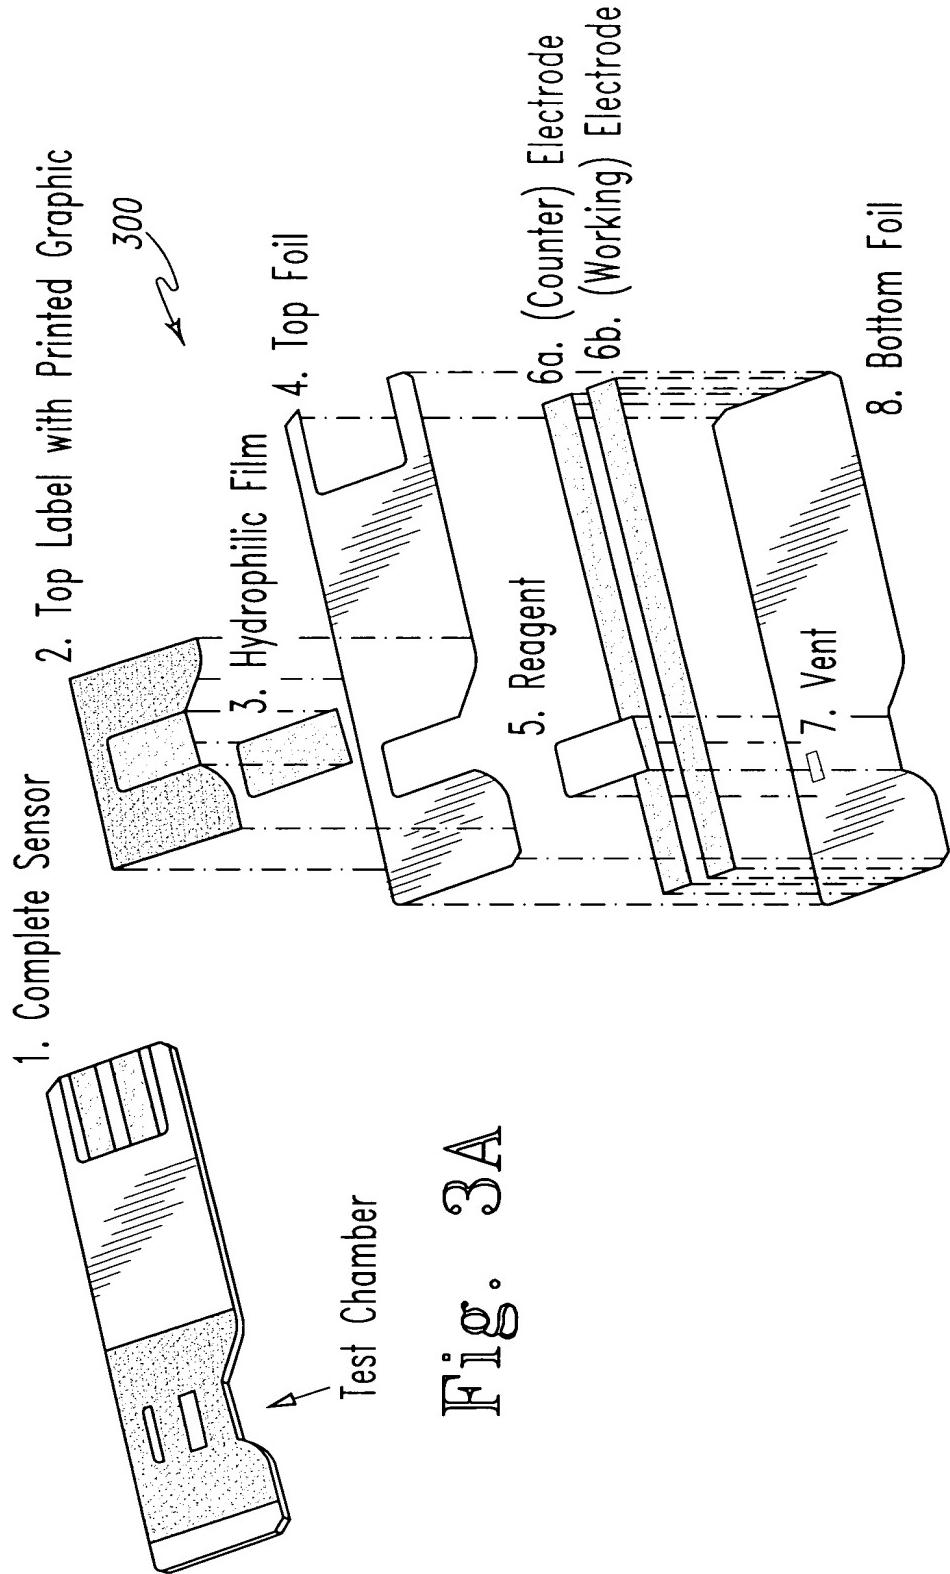

Serial No. Not Yet Assigned
Inventors: David W. Burke et al.
System and Method for Analyte Measurement
Employing Maximum Dosing Time Delay
Atty Docket: 7404-558

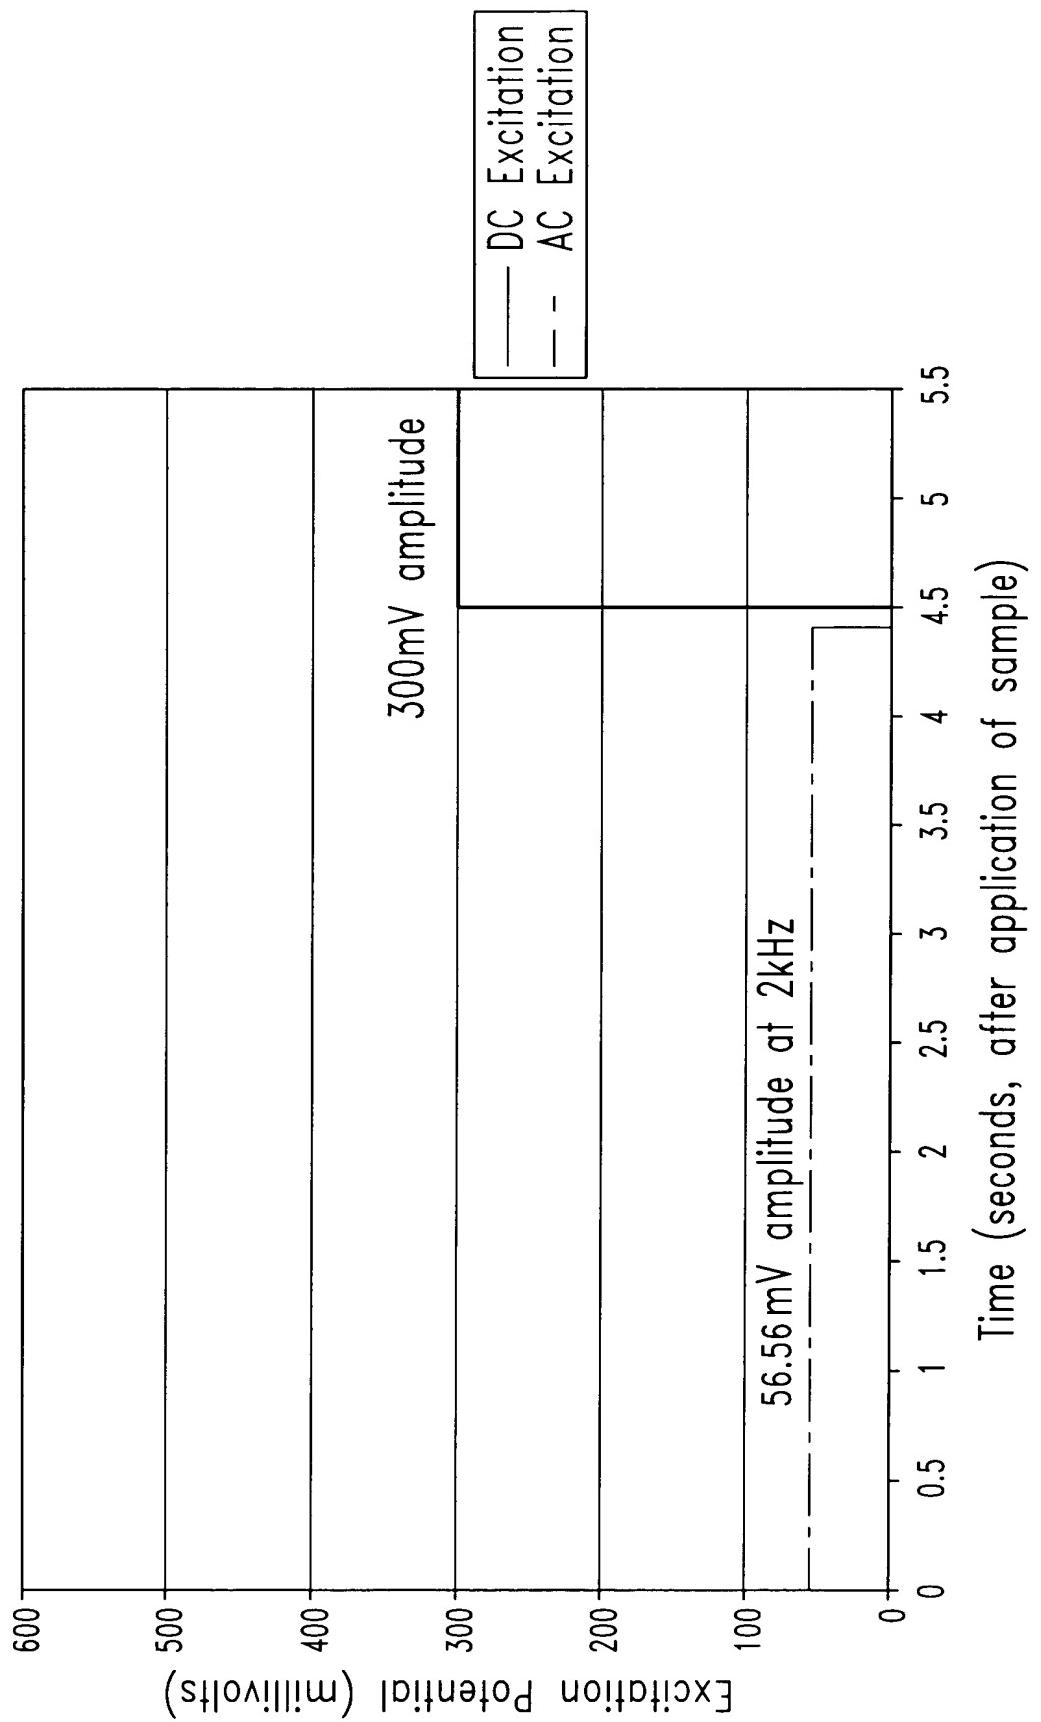


Fig. 4

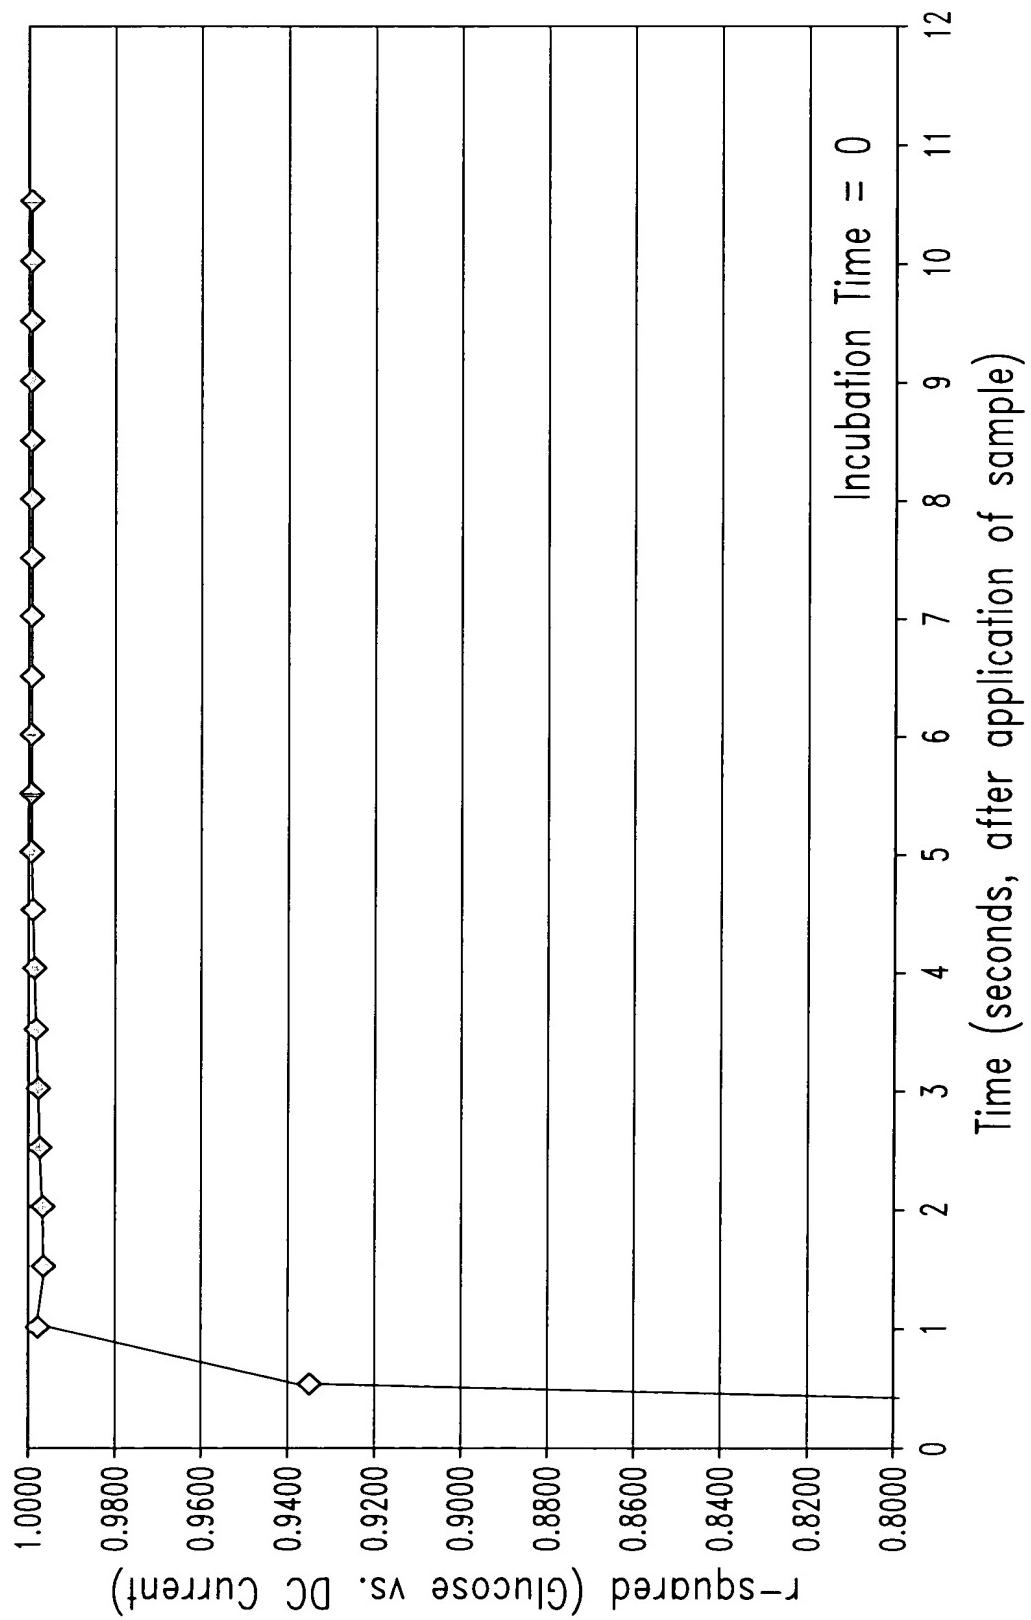


Fig. 5

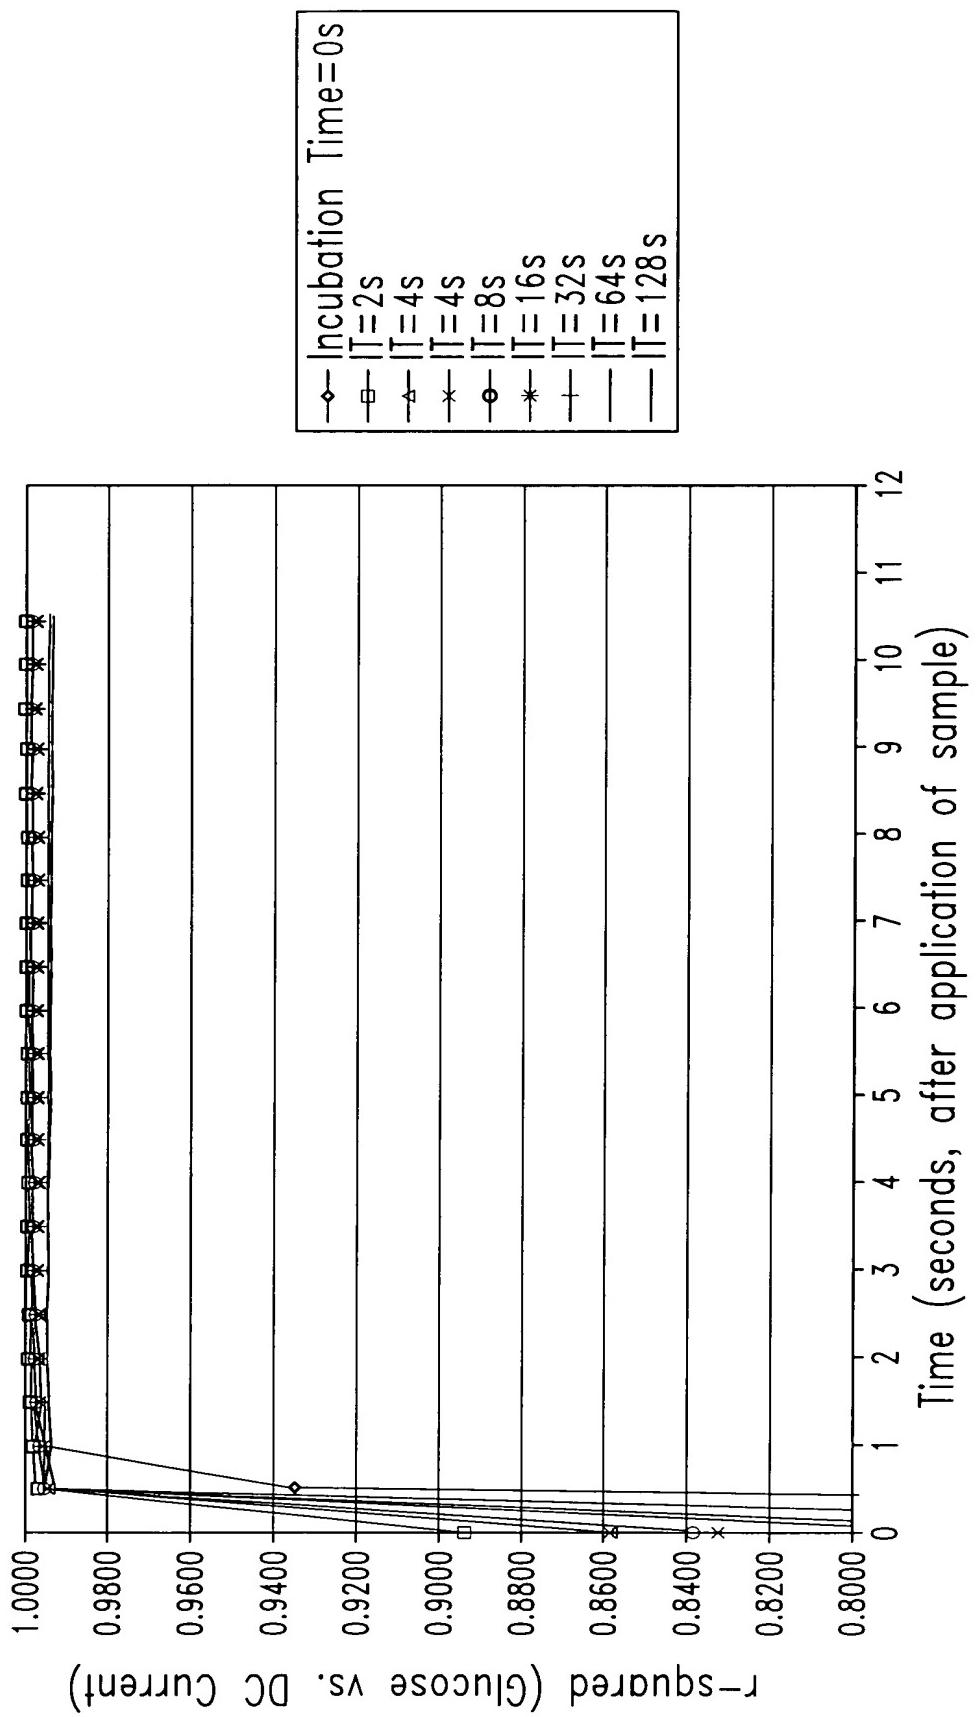


Fig. 6

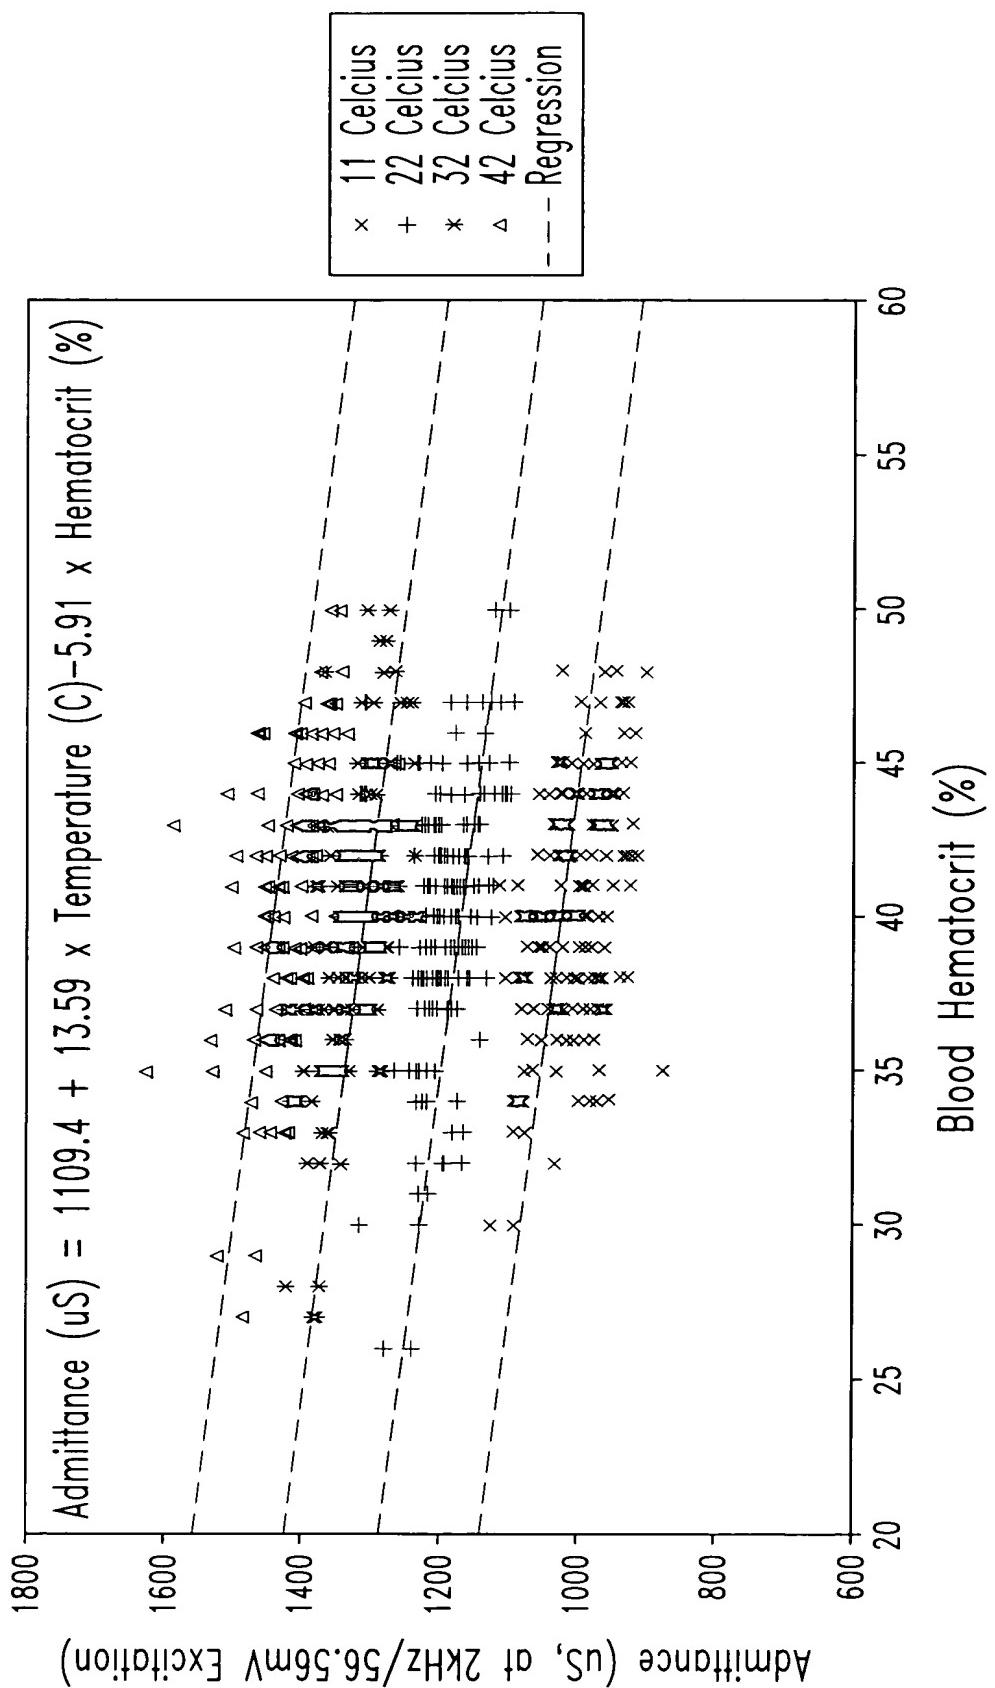


Fig. 7

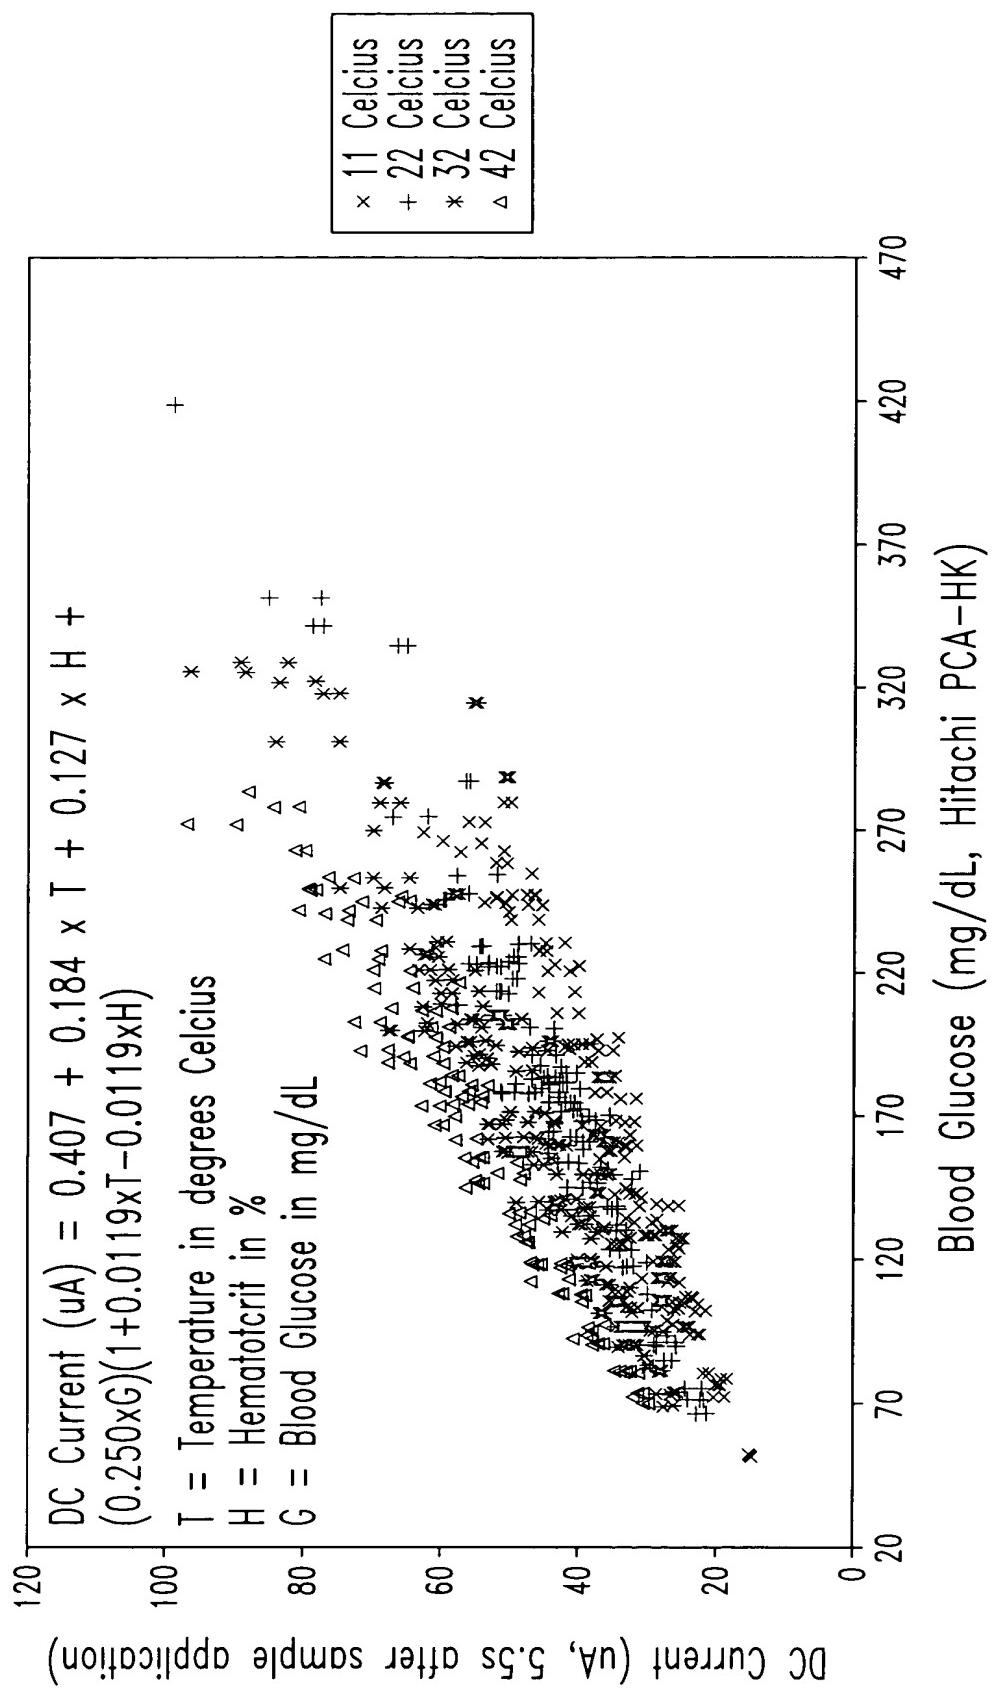


Fig. 8

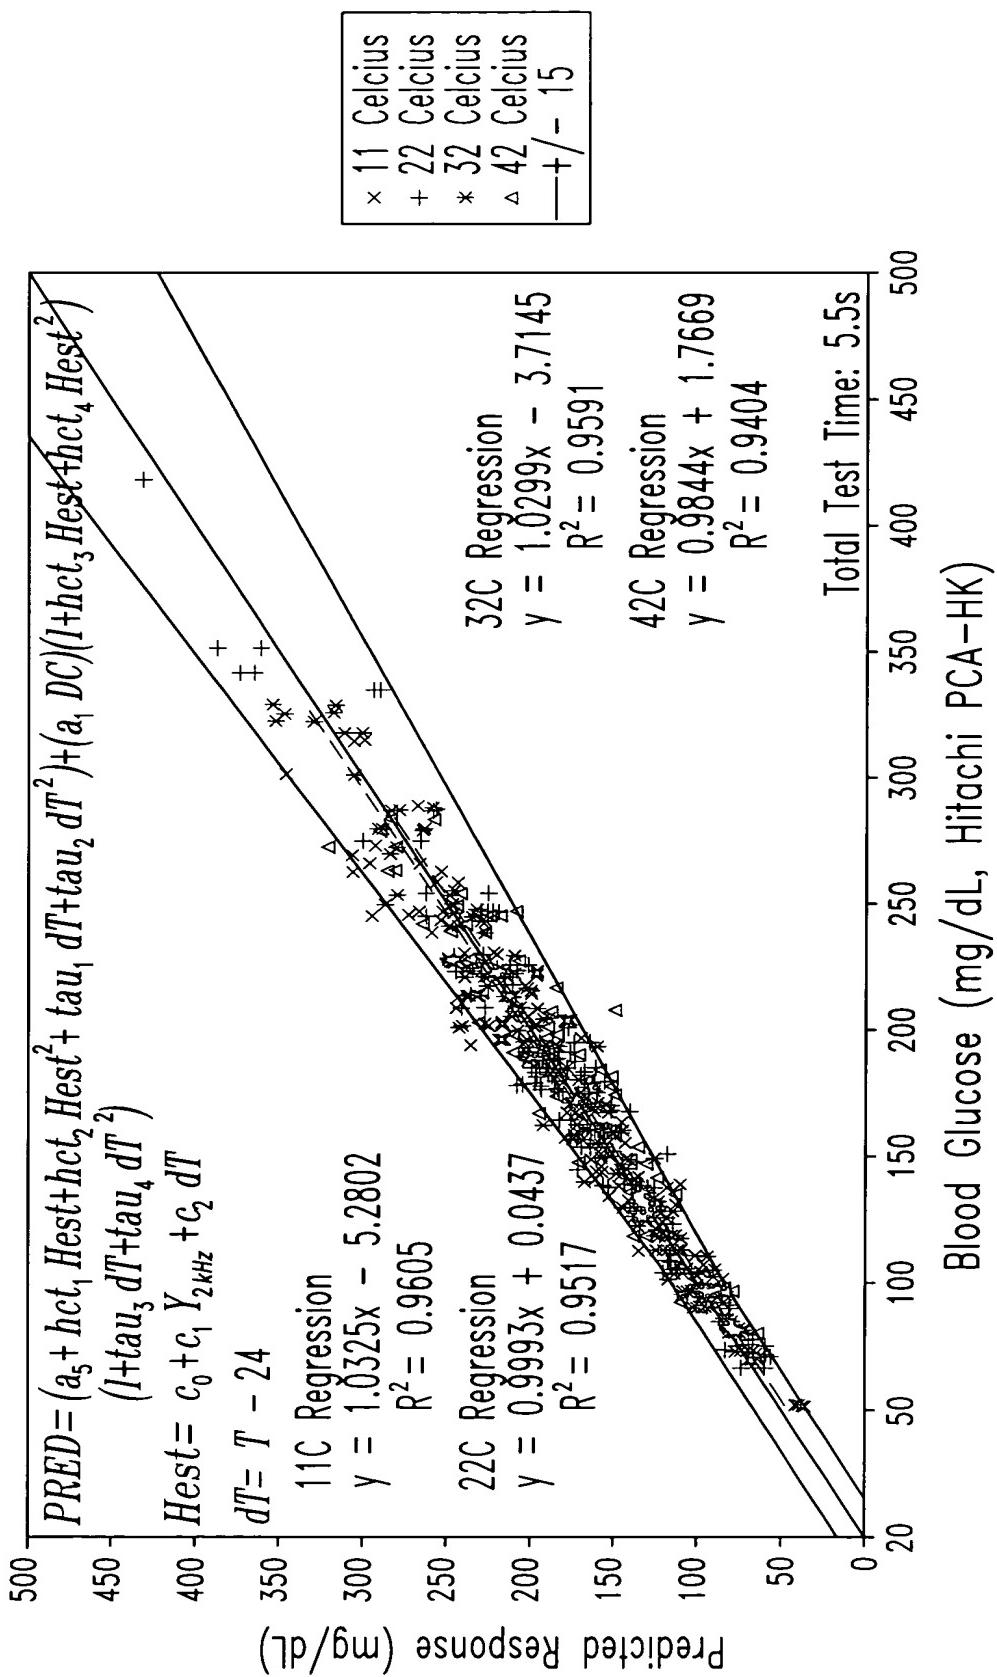


Fig. 9

Serial No. Not Yet Assigned
Inventors: David W. Burke et al.
System and Method for Analyte Measurement
Employing Maximum Dosing Time Delay
Atty Docket: 7404-558

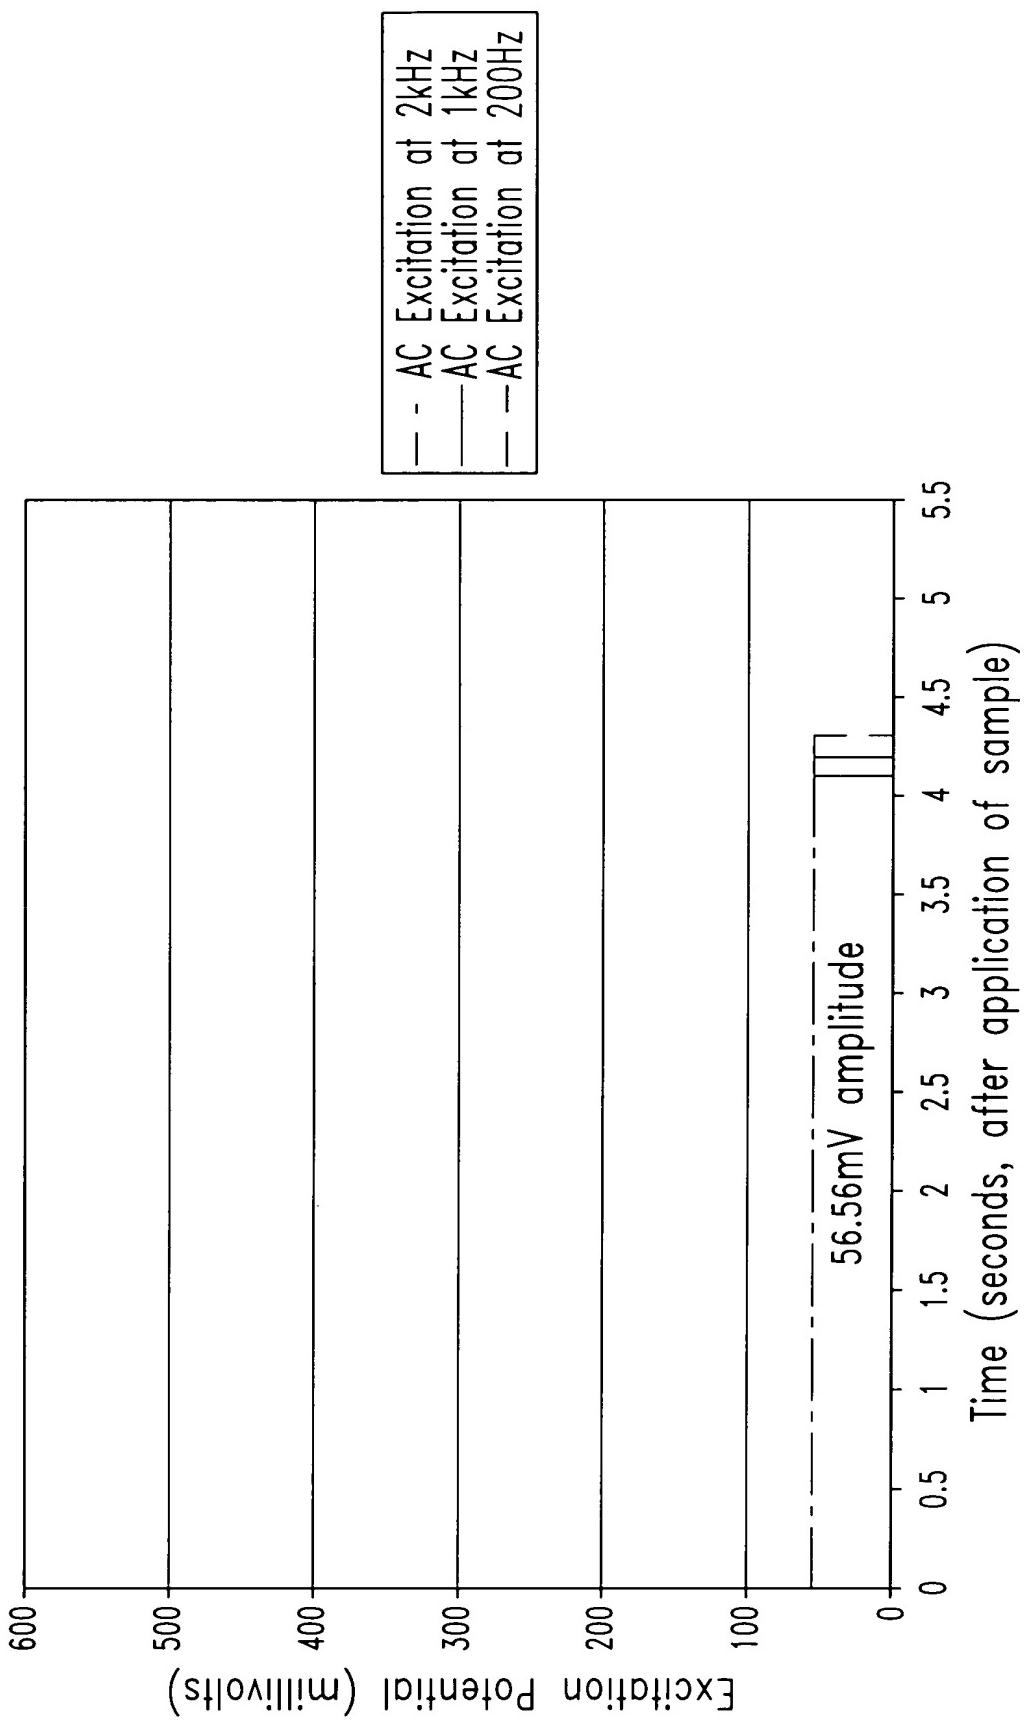


Fig. 10

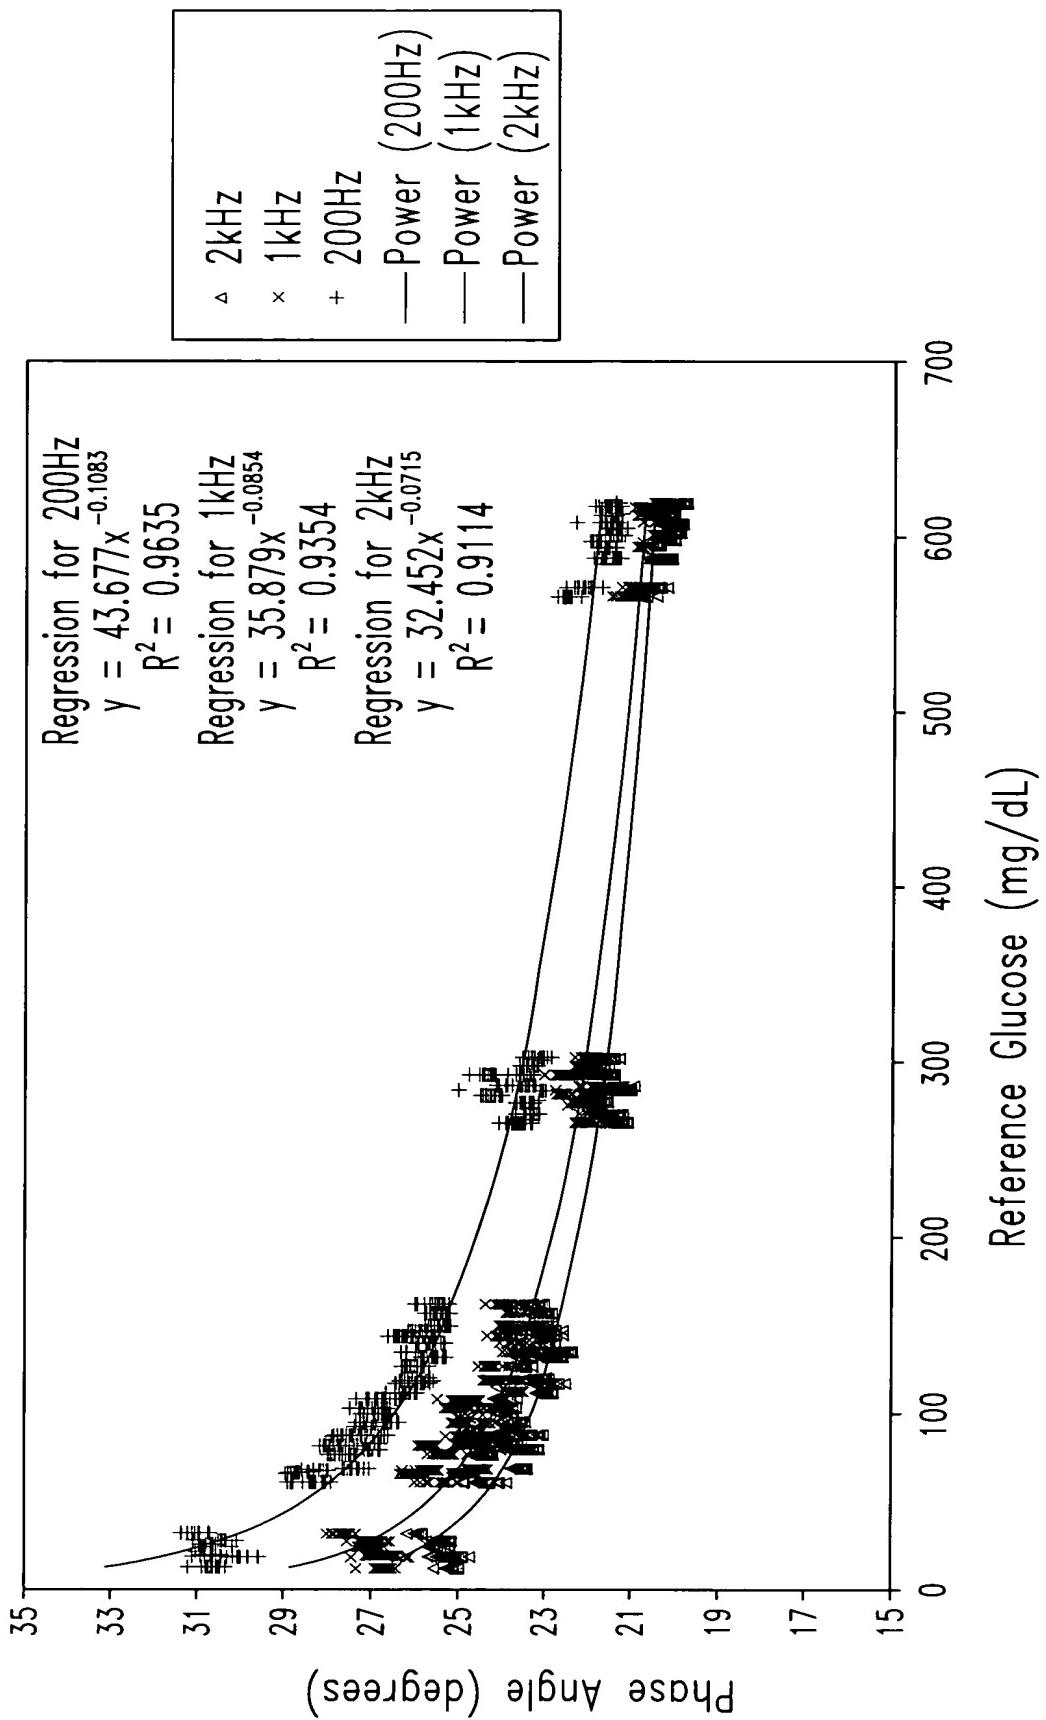


Fig. 11

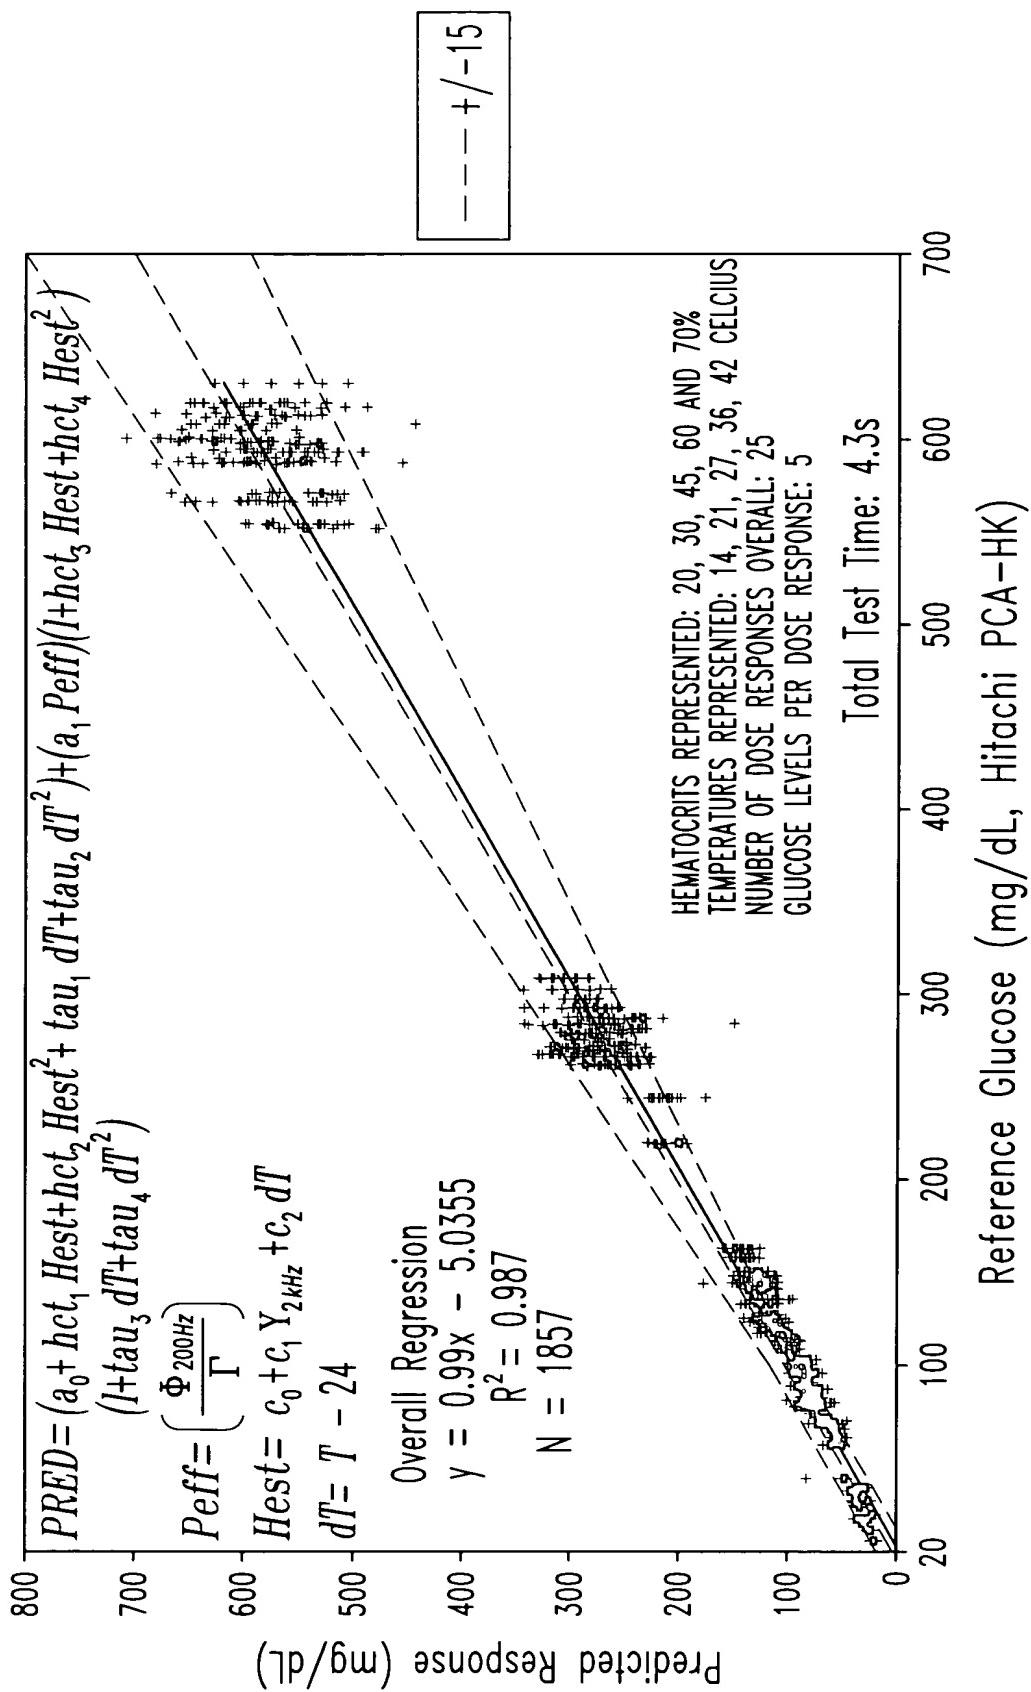


Fig. 12

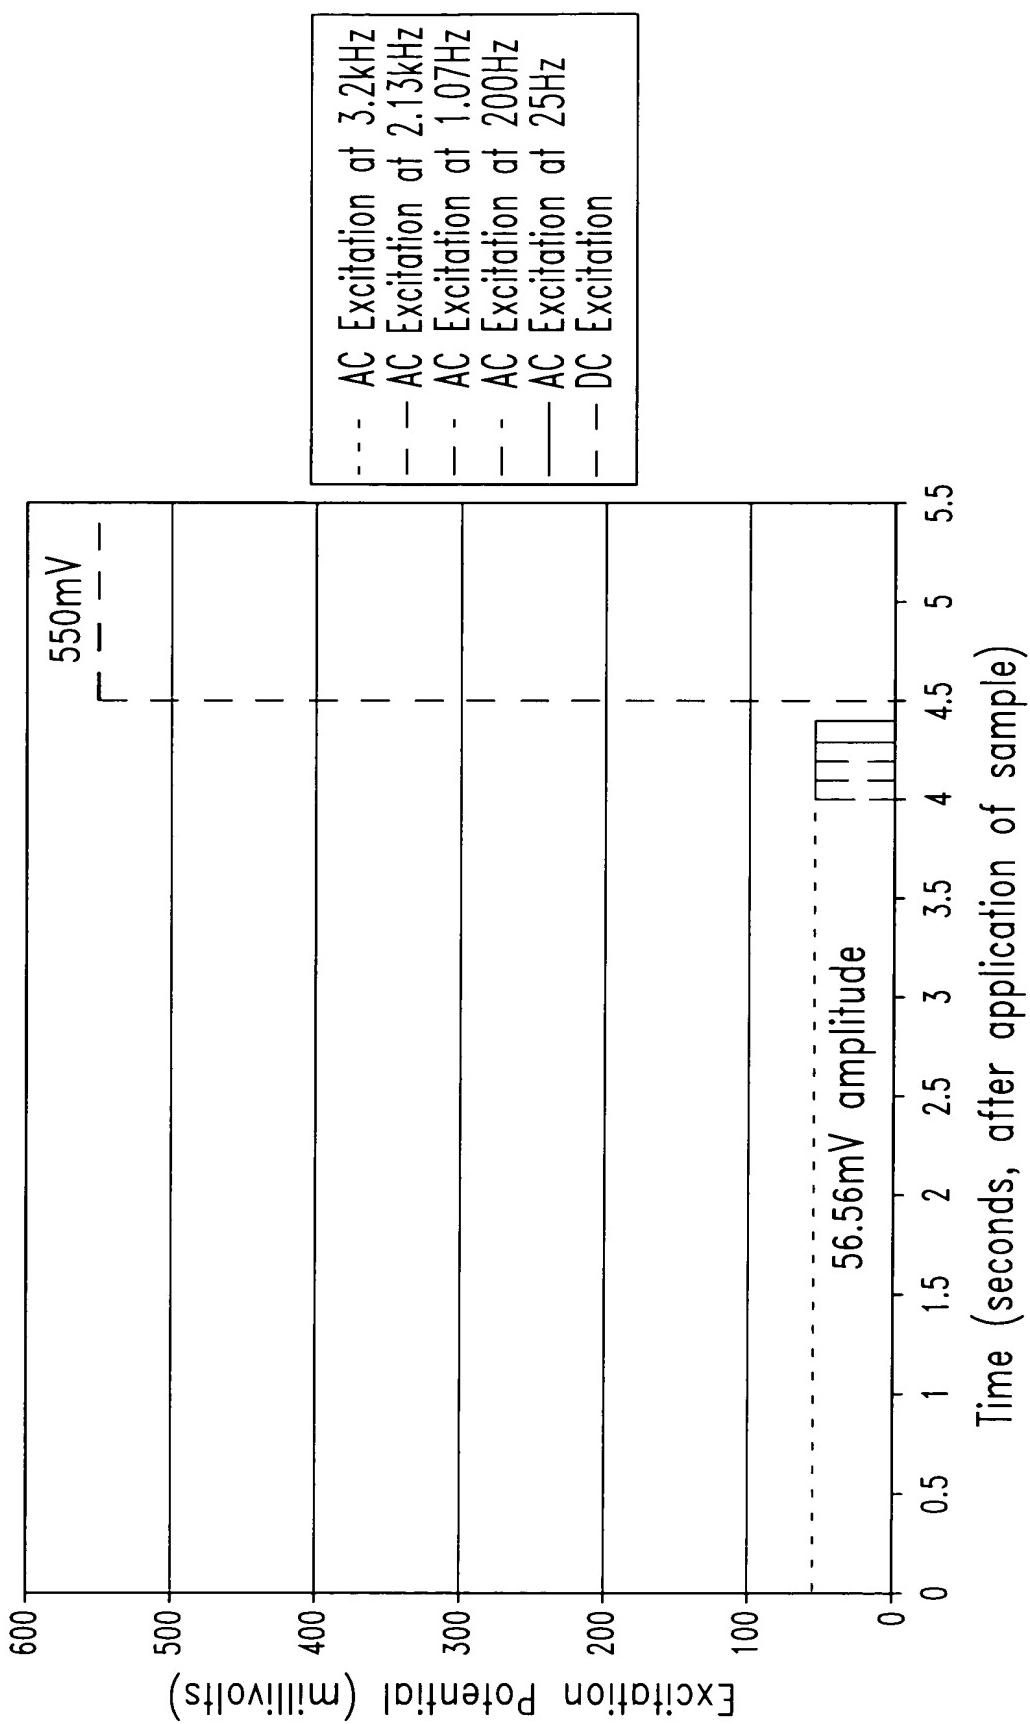


Fig. 13

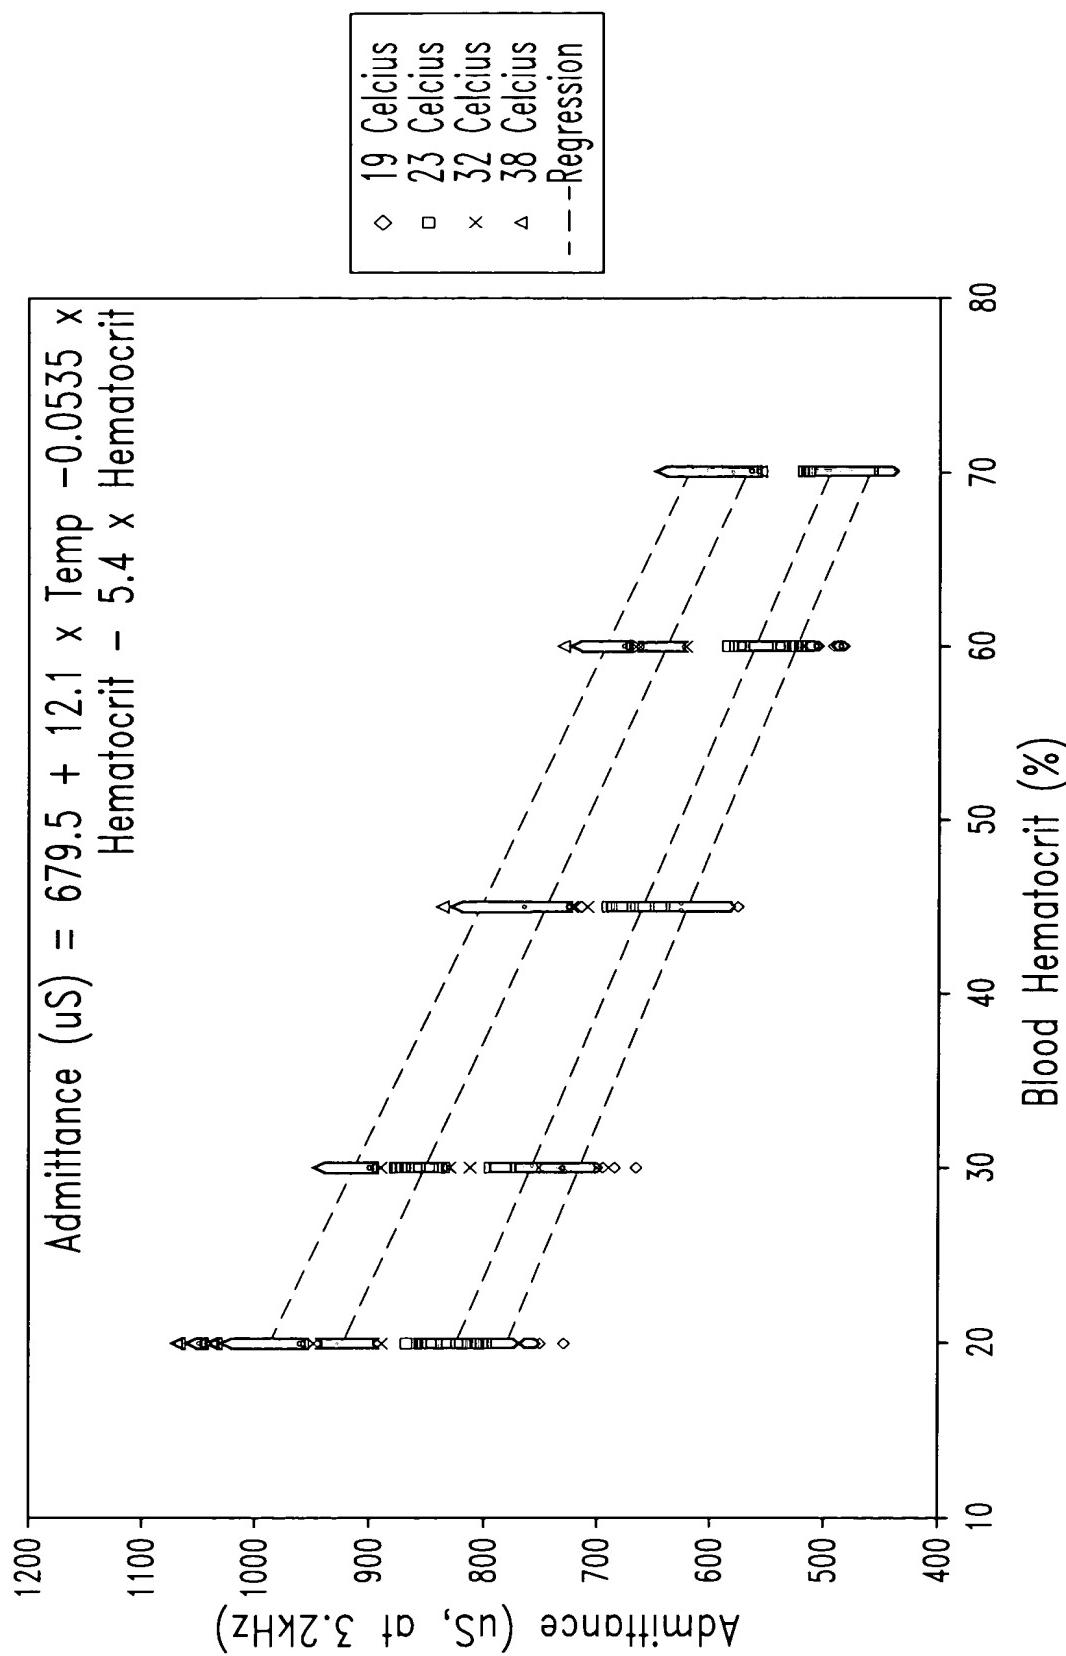


Fig. 14

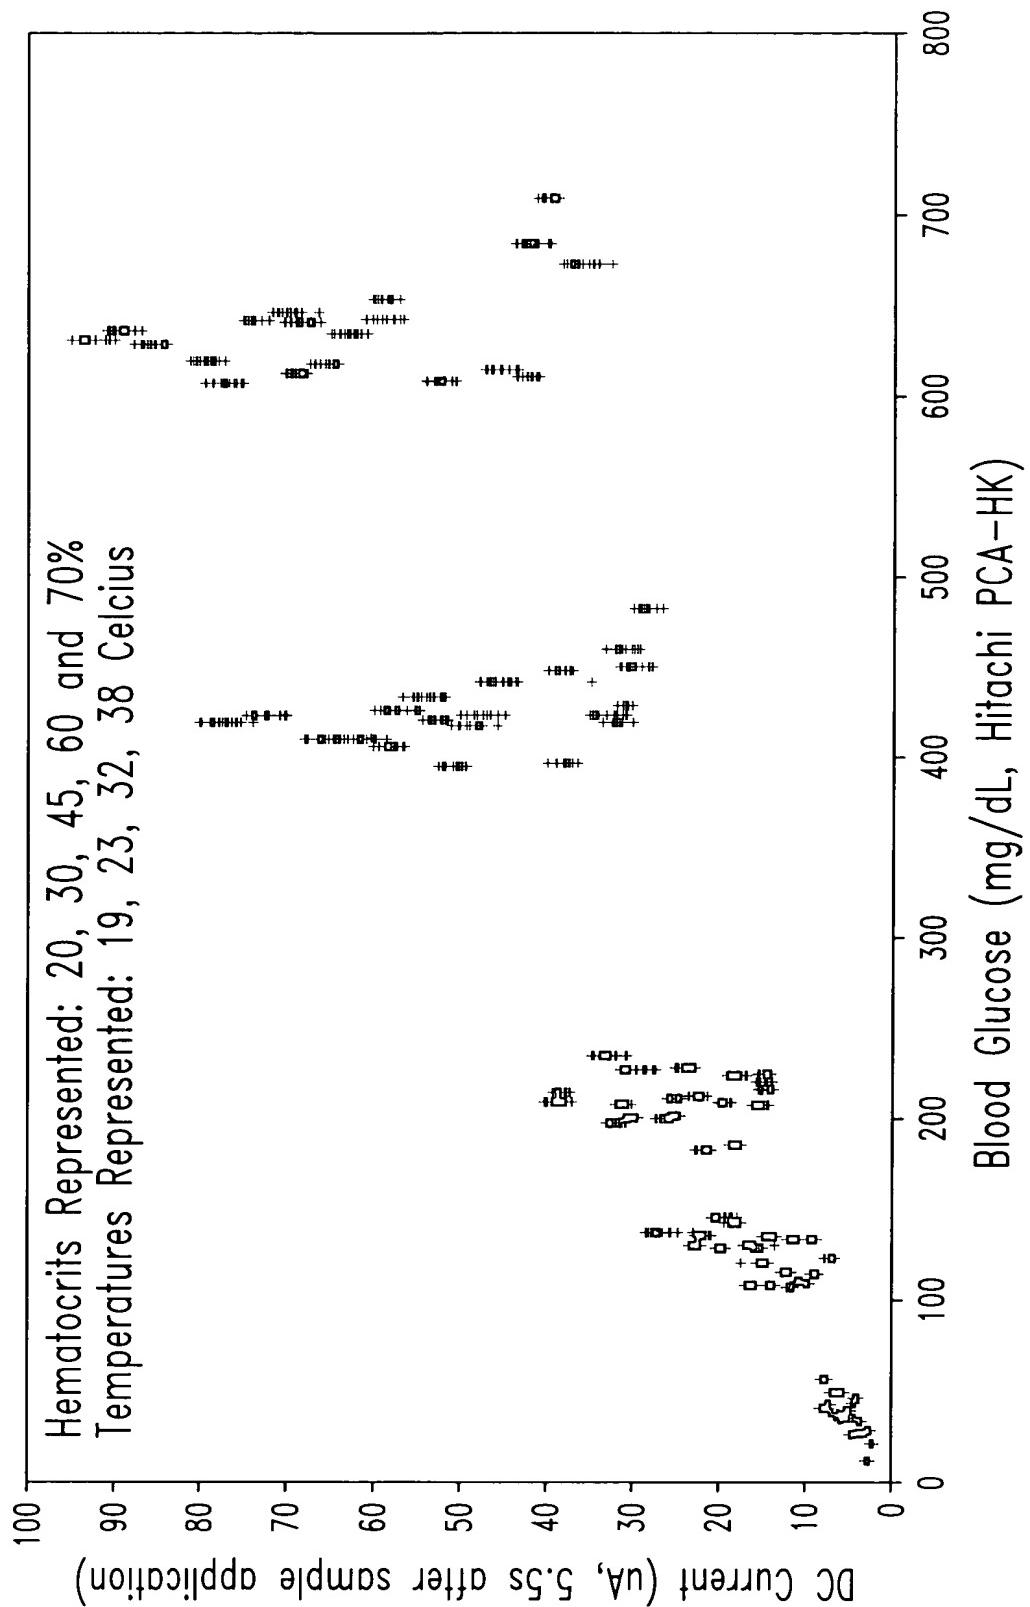


Fig. 15

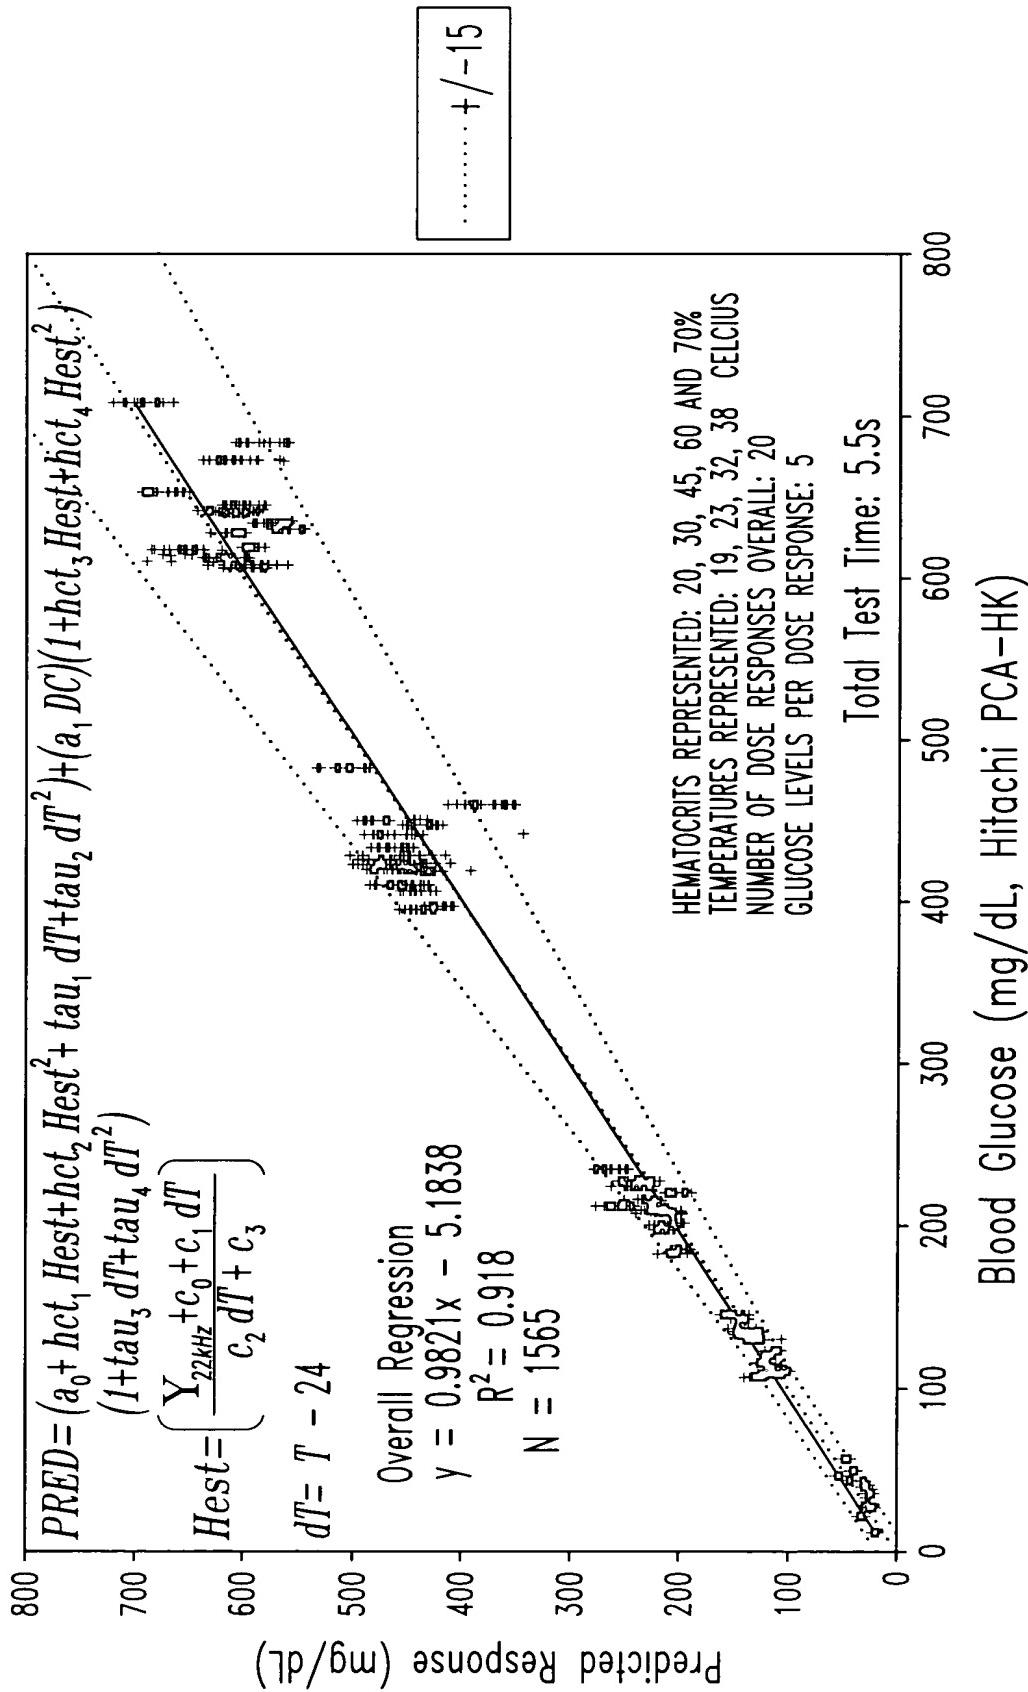


Fig. 16

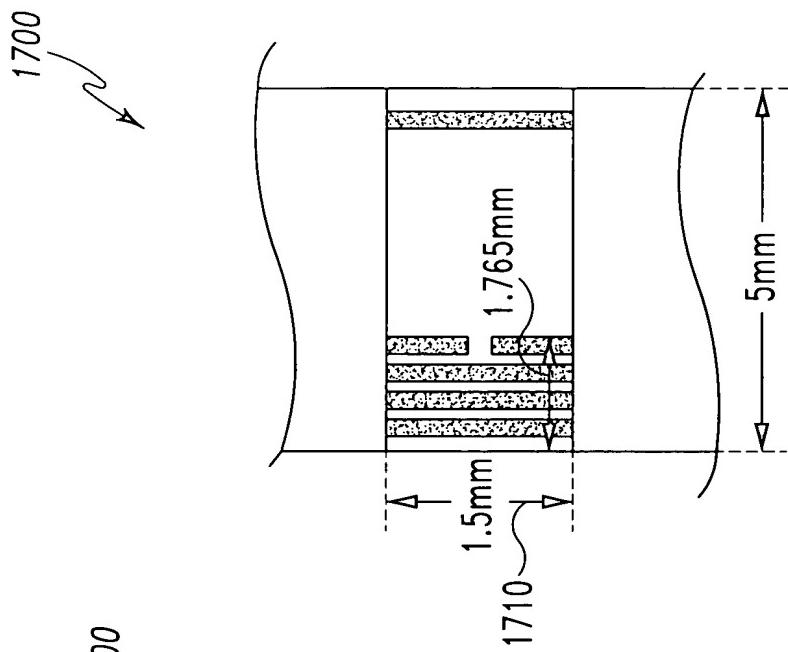


Fig. 17B

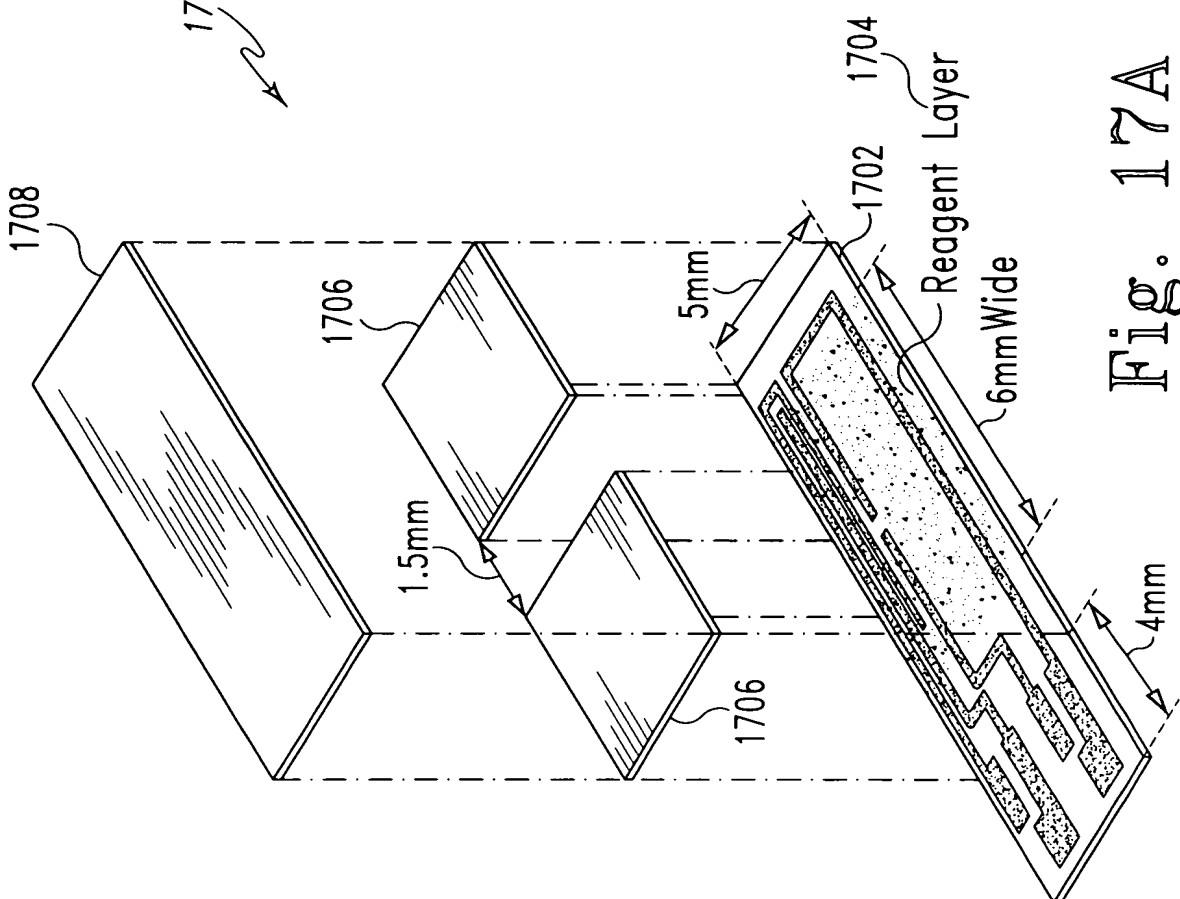


Fig. 17A

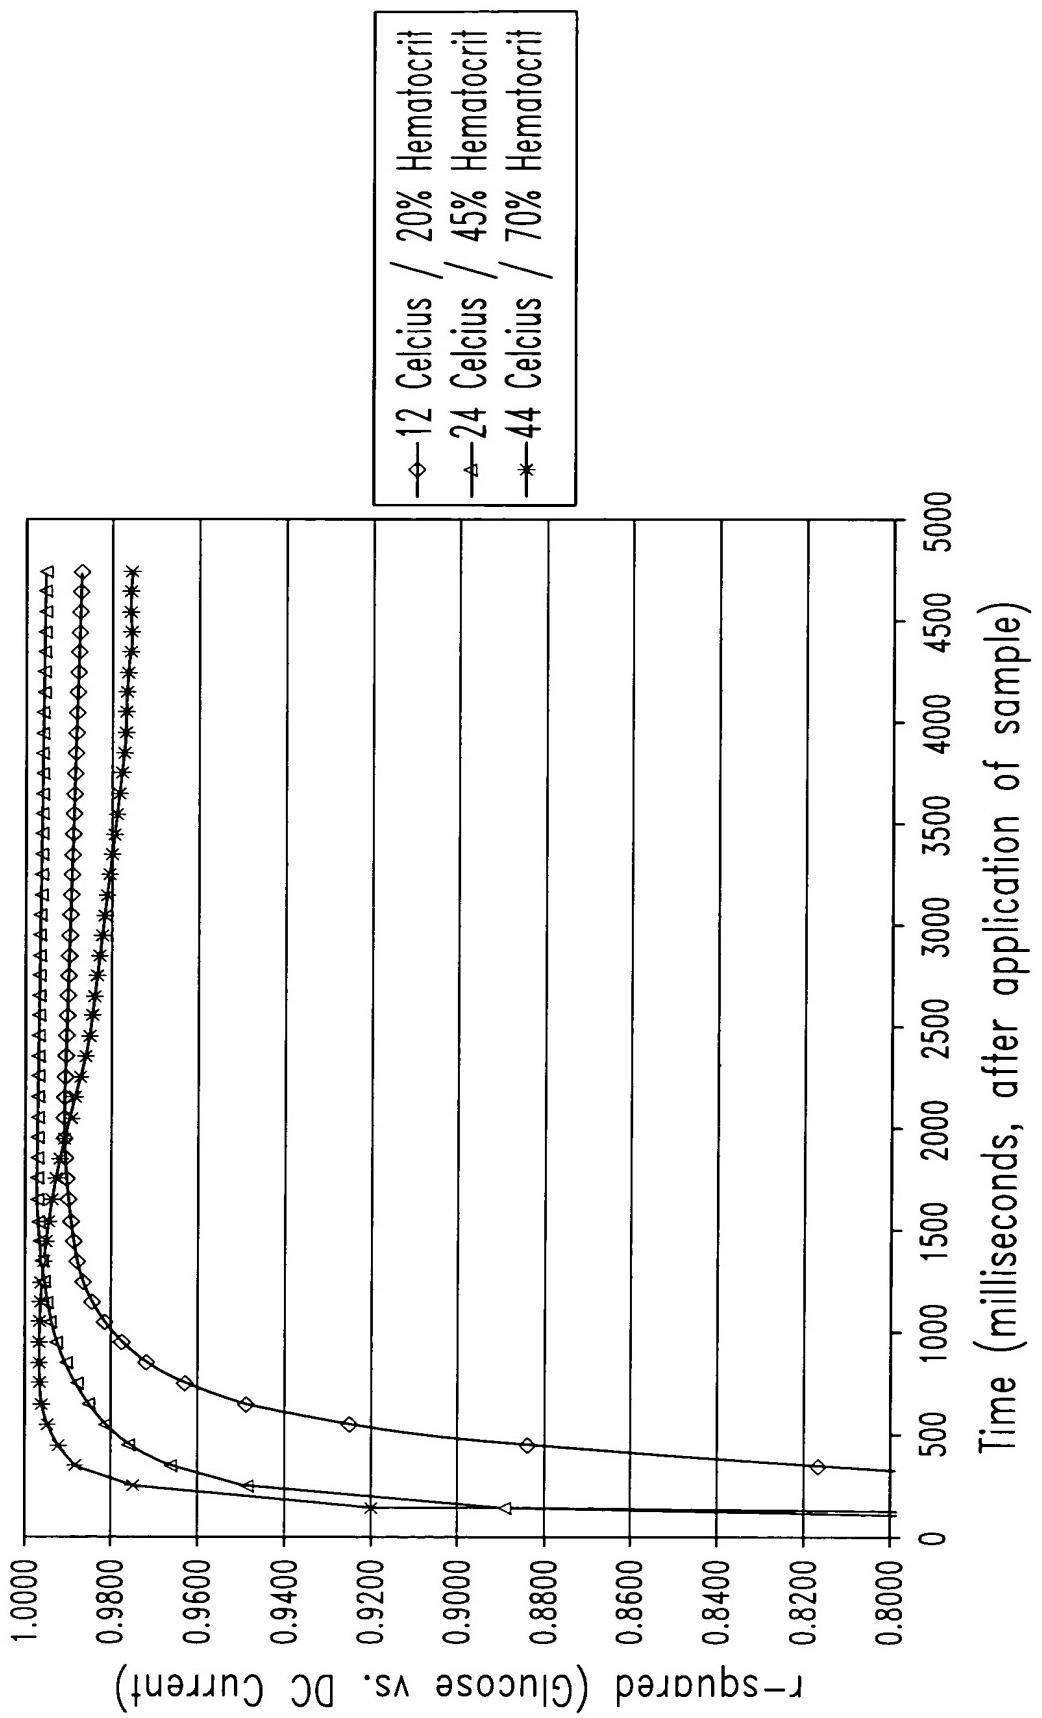


Fig. 18

Serial No. Not Yet Assigned
Inventors: David W. Burke et al.
System and Method for Analyte Measurement
Employing Maximum Dosing Time Delay
Atty Docket: 7404-558

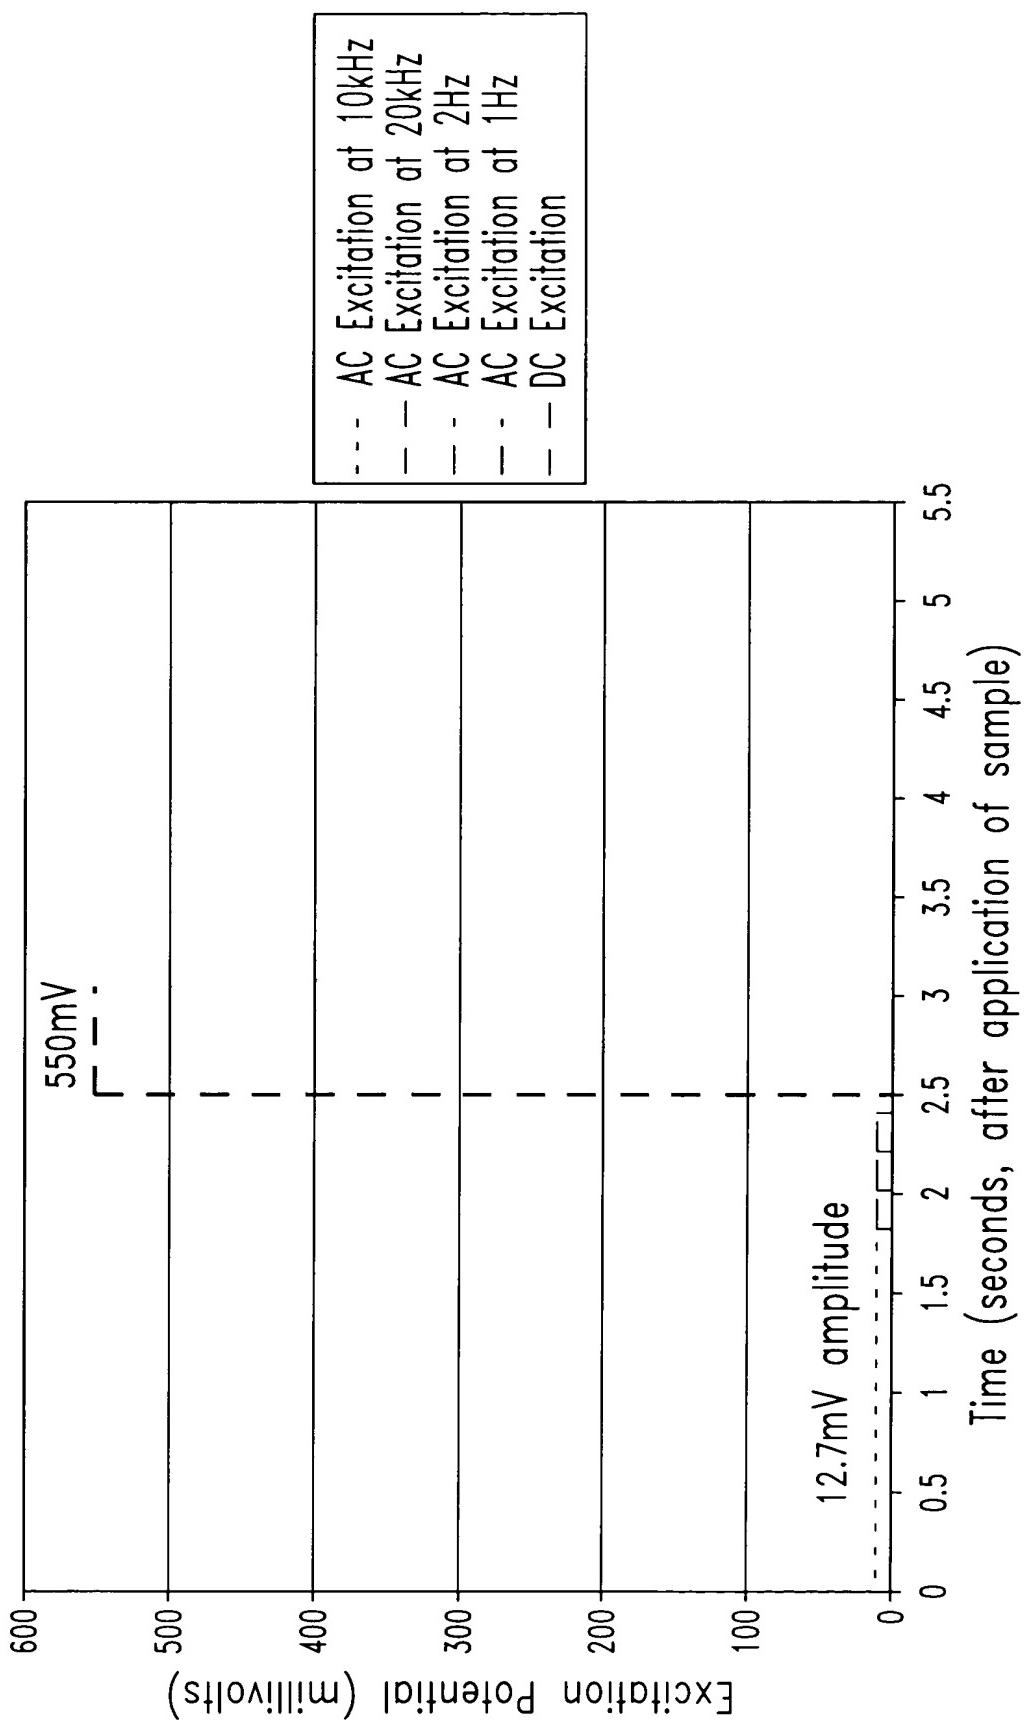


Fig. 19

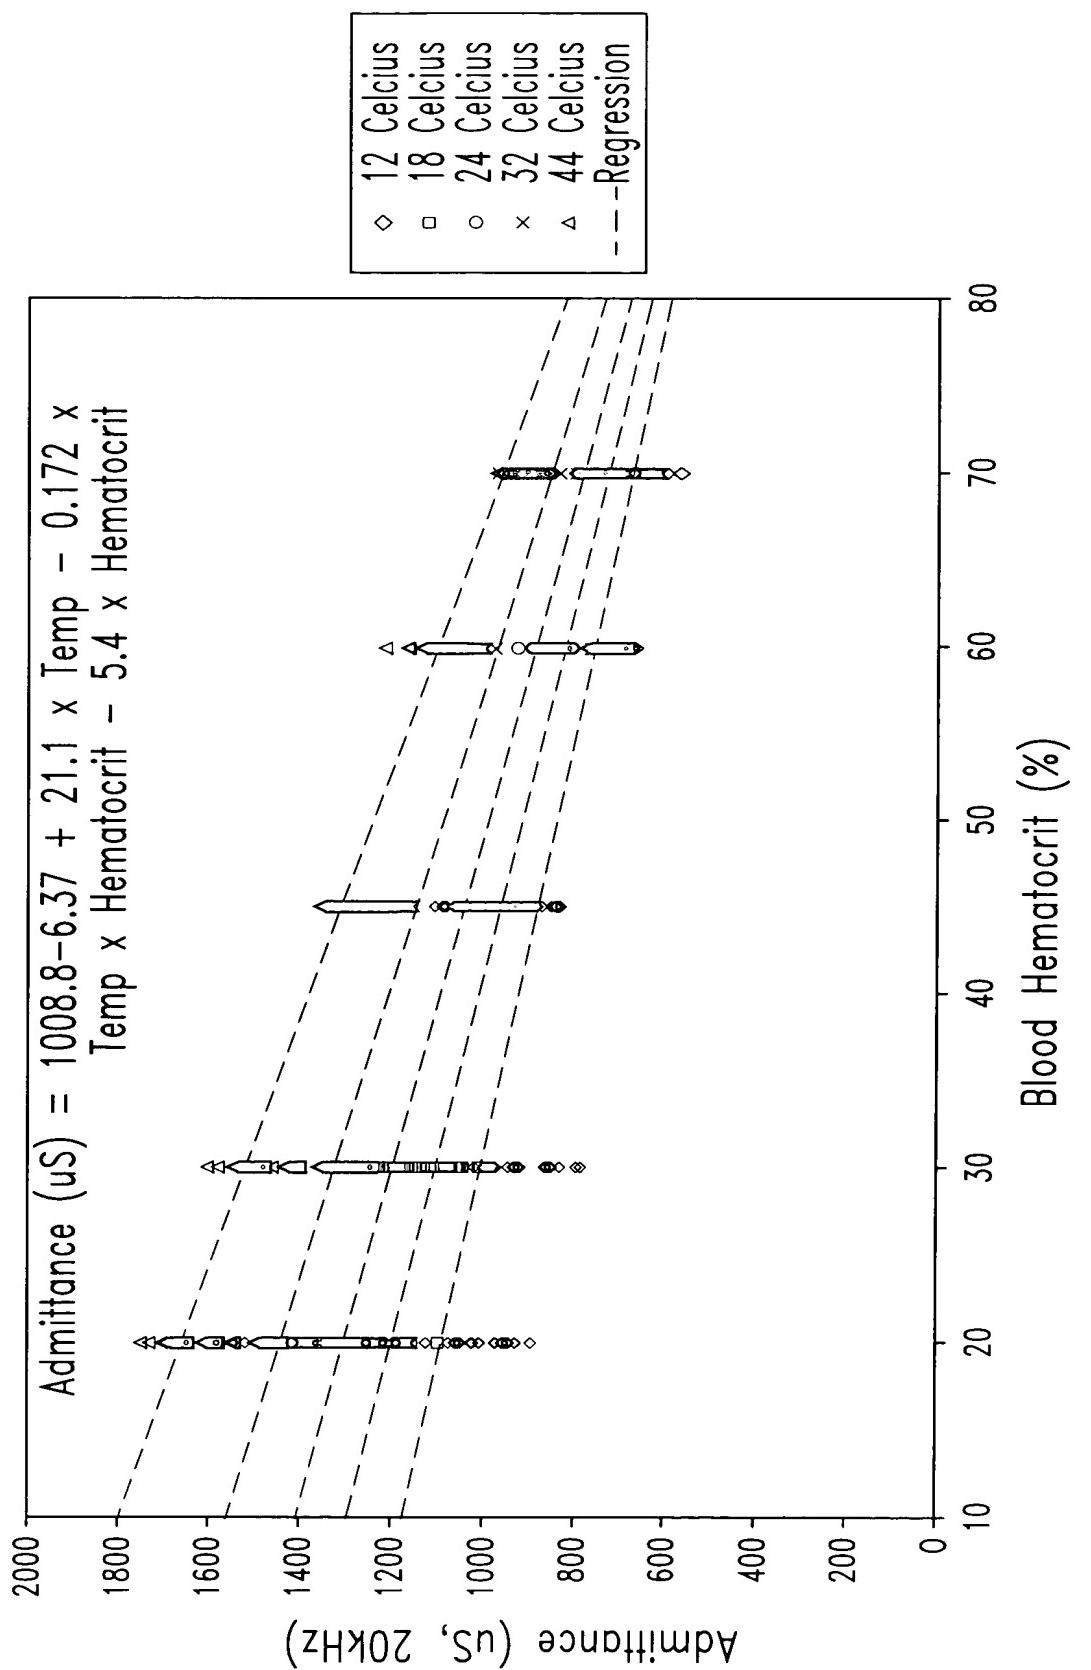


Fig. 20

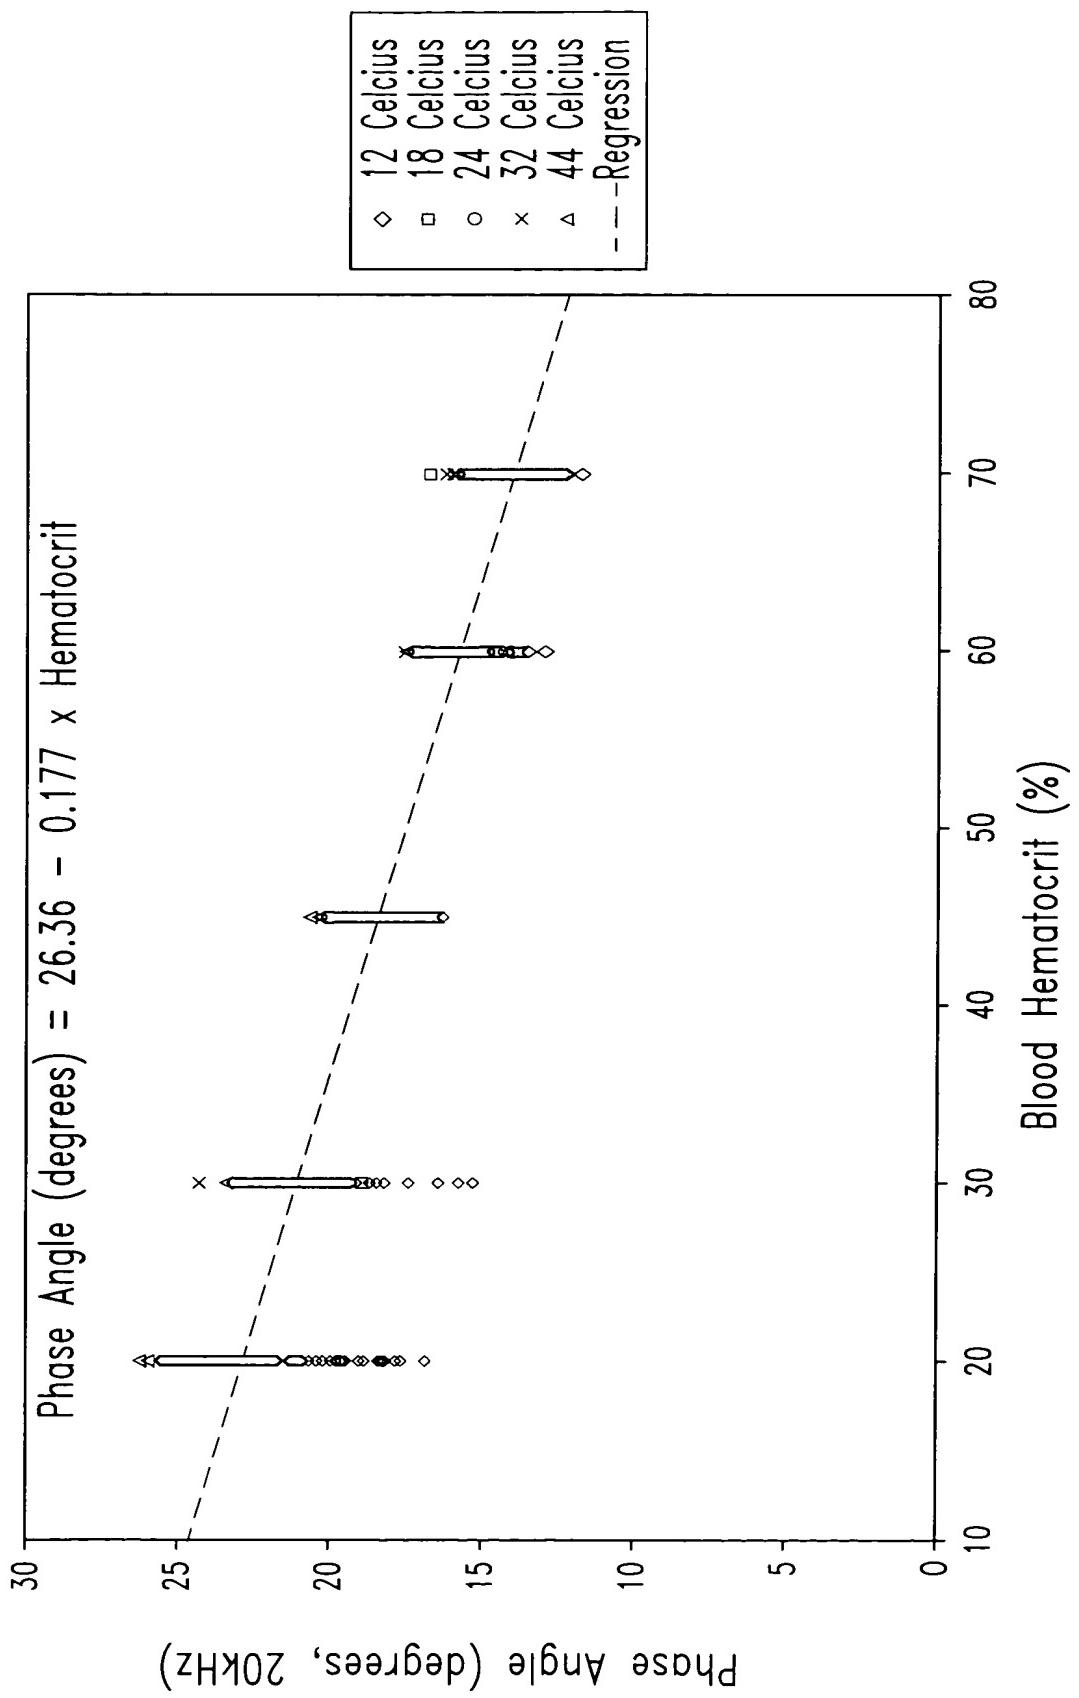


Fig. 21

Serial No. Not Yet Assigned
Inventors: David W. Burke et al.
System and Method for Analyte Measurement
Employing Maximum Dosing Time Delay
Atty Docket: 7404-558

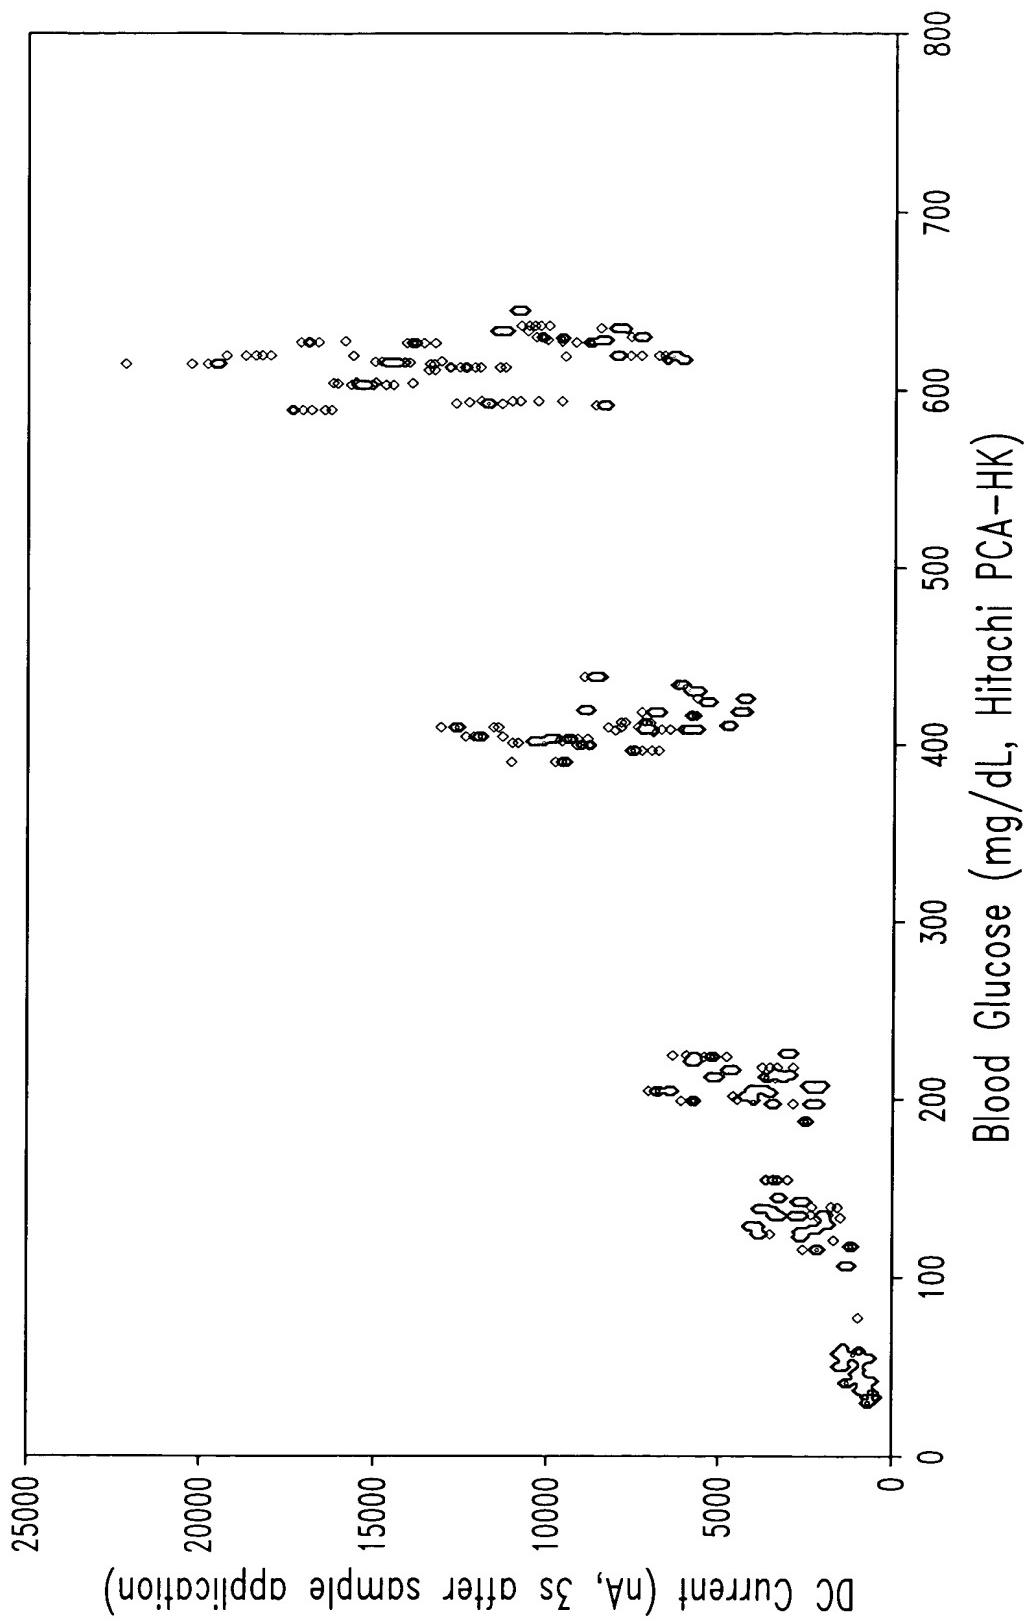


Fig. 22

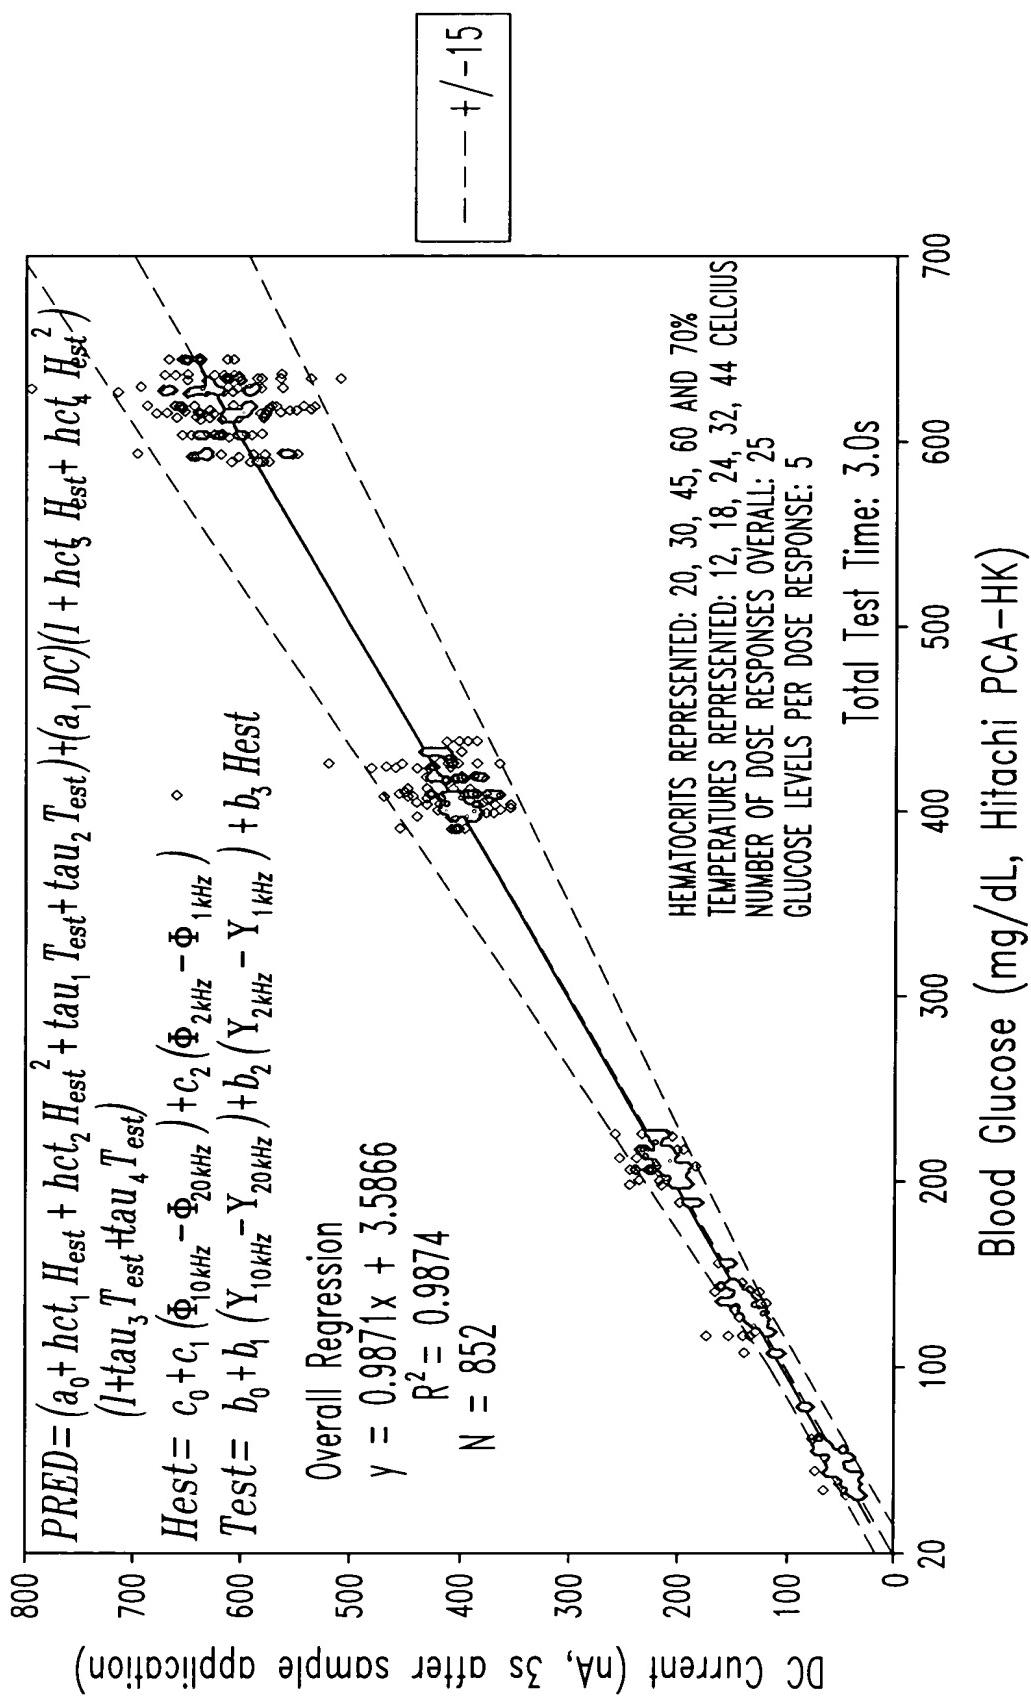


Fig. 23

Serial No. Not Yet Assigned
Inventors: David W. Burke et al.
System and Method for Analyte Measurement
Employing Maximum Dosing Time Delay
Atty Docket: 7404-558

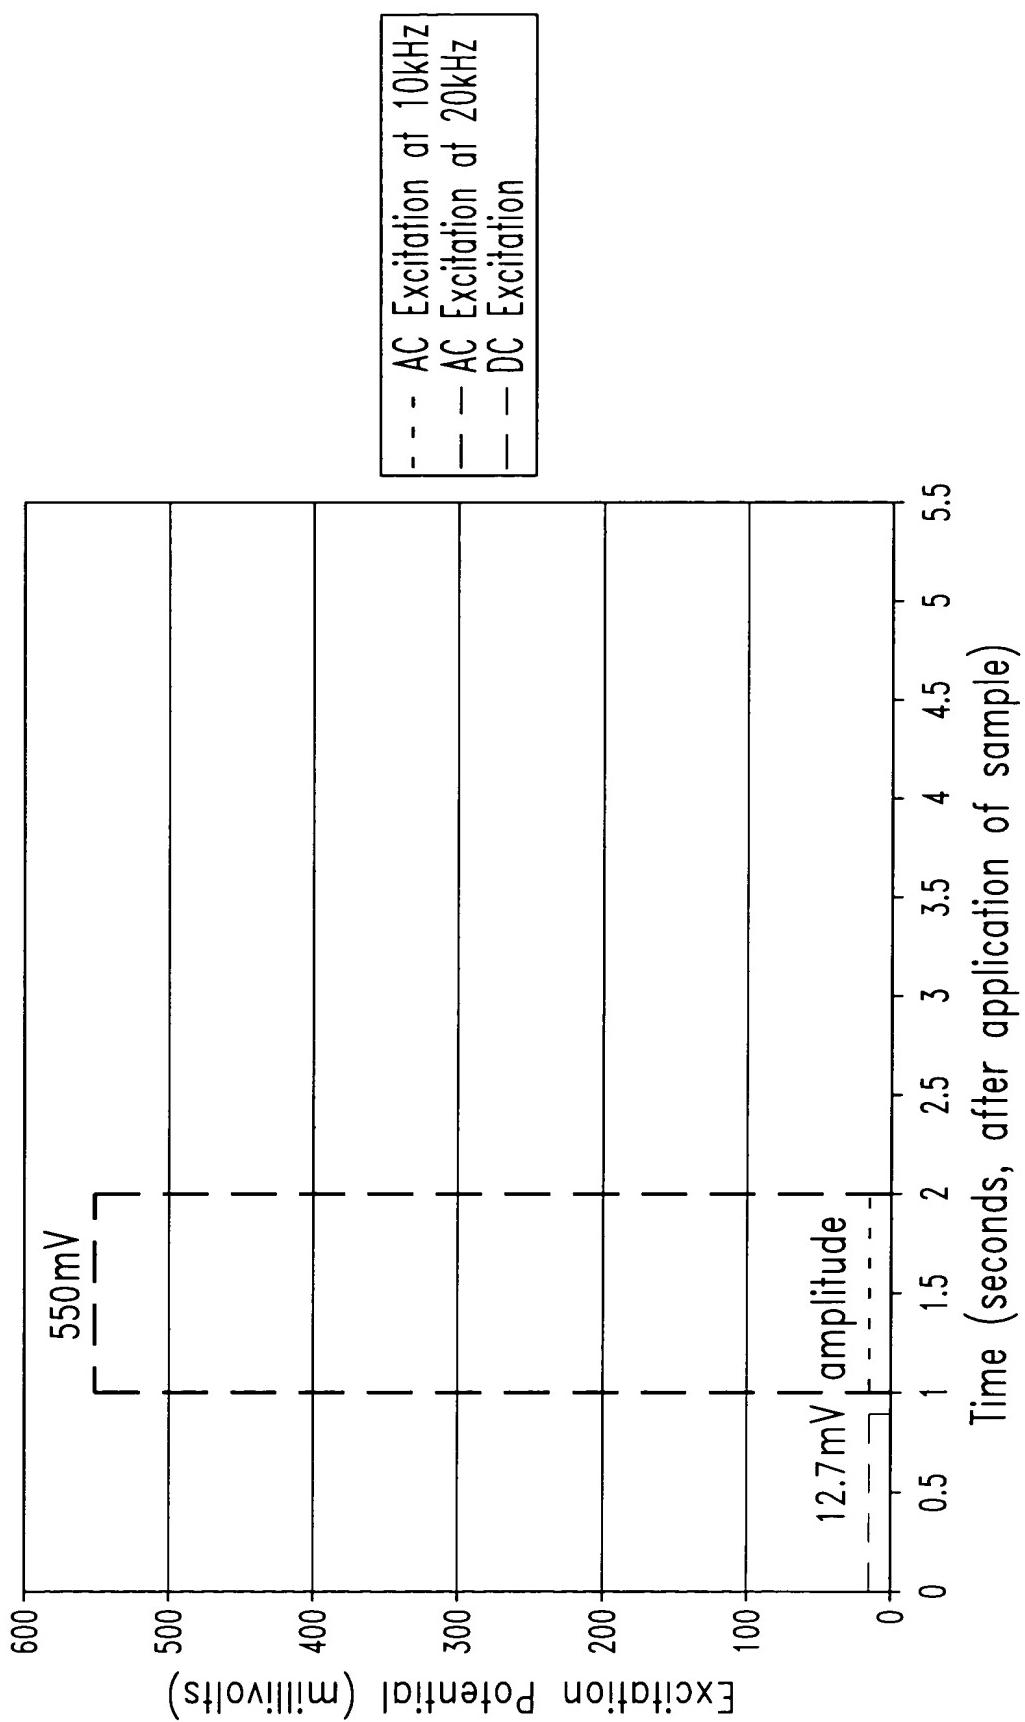


Fig. 24

Serial No. Not Yet Assigned
Inventors: David W. Burke et al.
System and Method for Analyte Measurement
Employing Maximum Dosing Time Delay
Atty Docket: 7404-558

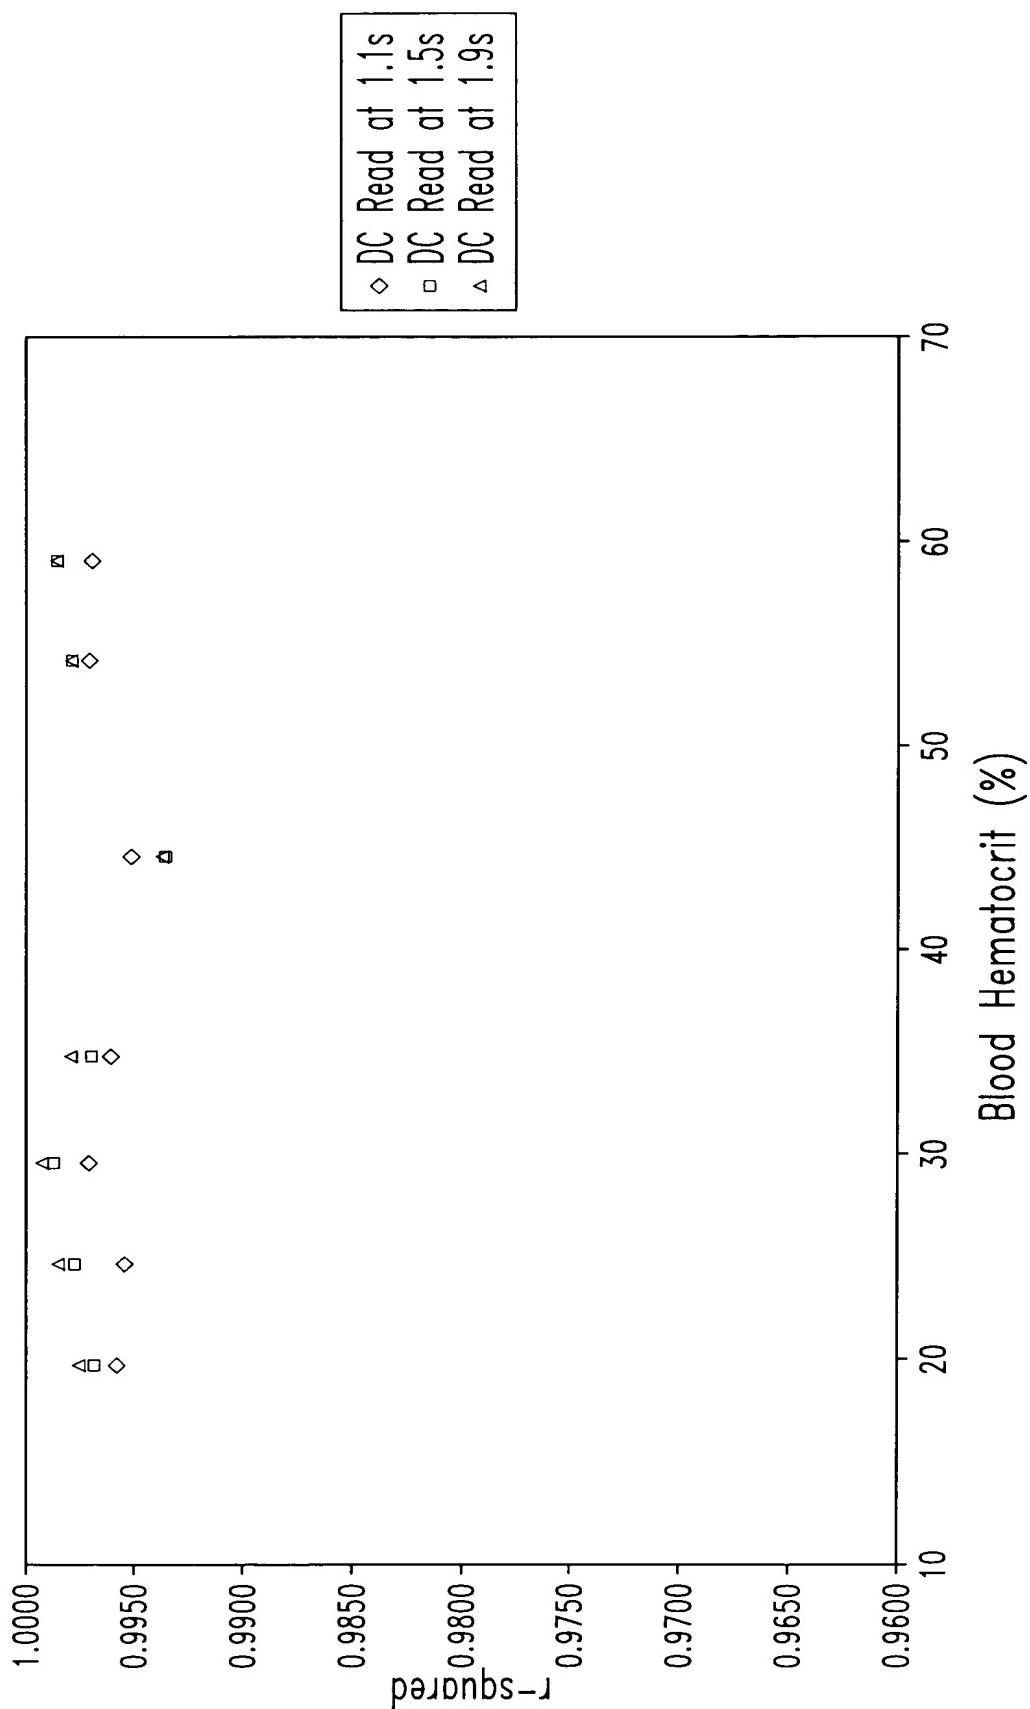


Fig. 25

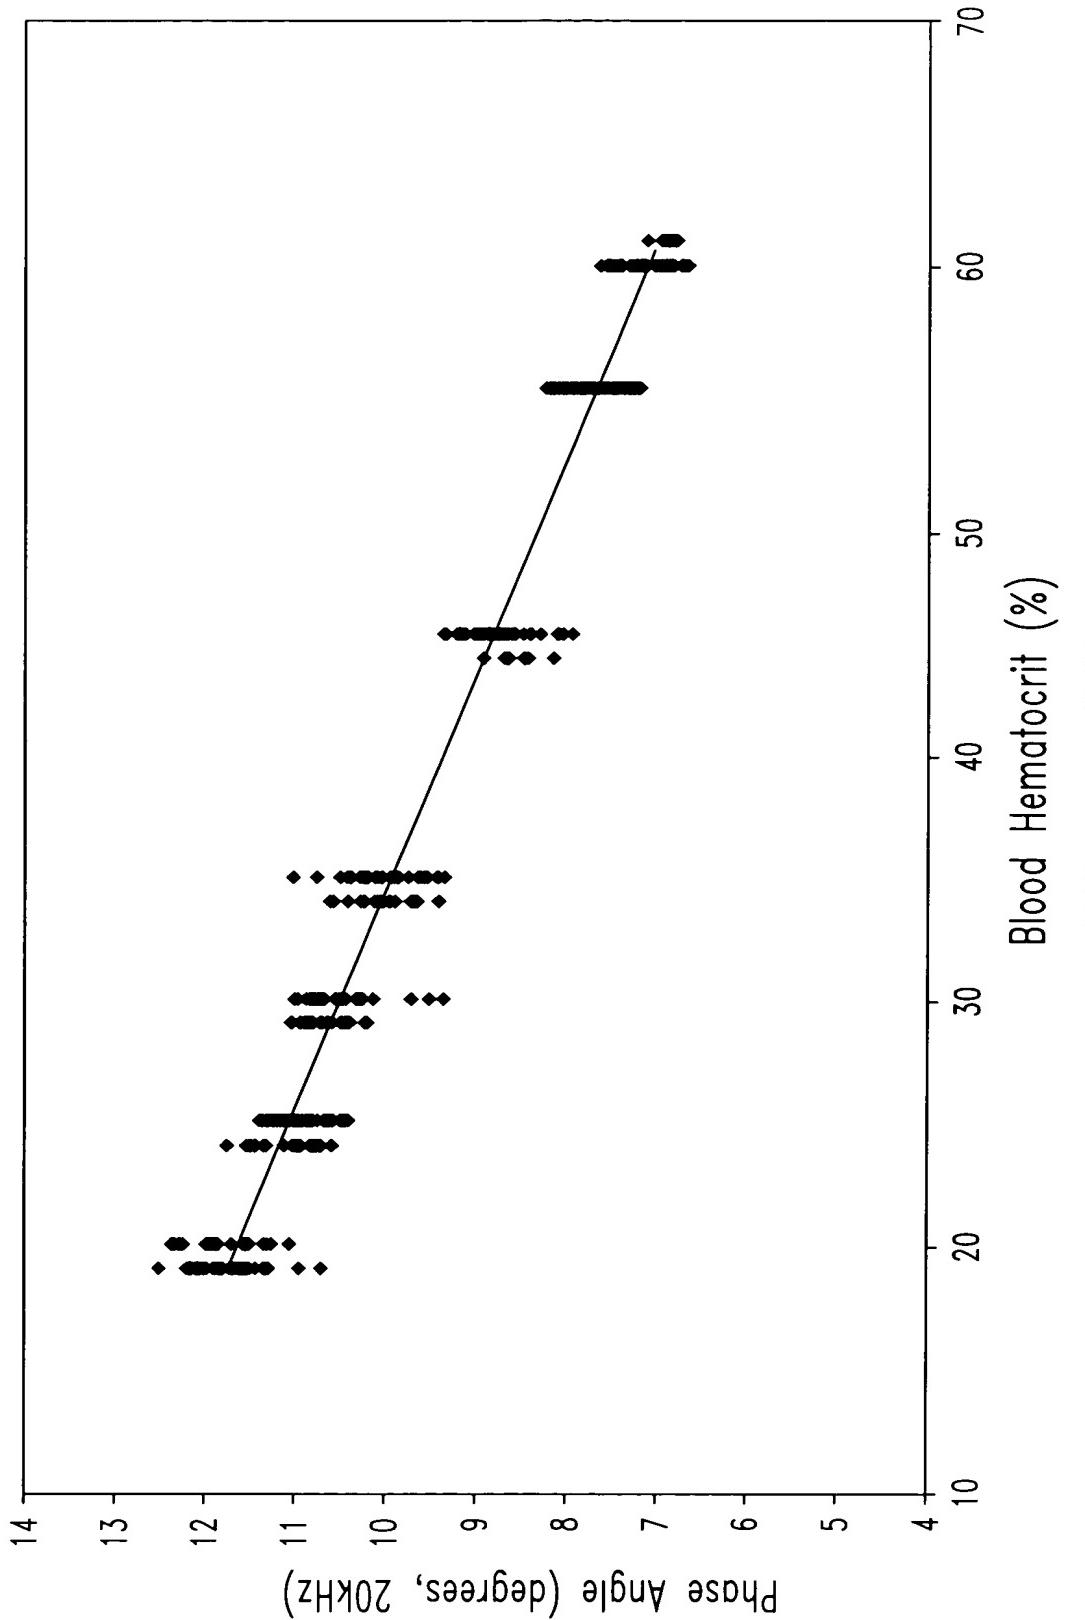


Fig. 26

Serial No. Not Yet Assigned
Inventors: David W. Burke et al.
System and Method for Analyte Measurement
Employing Maximum Dosing Time Delay
Atty Docket: 7404-558

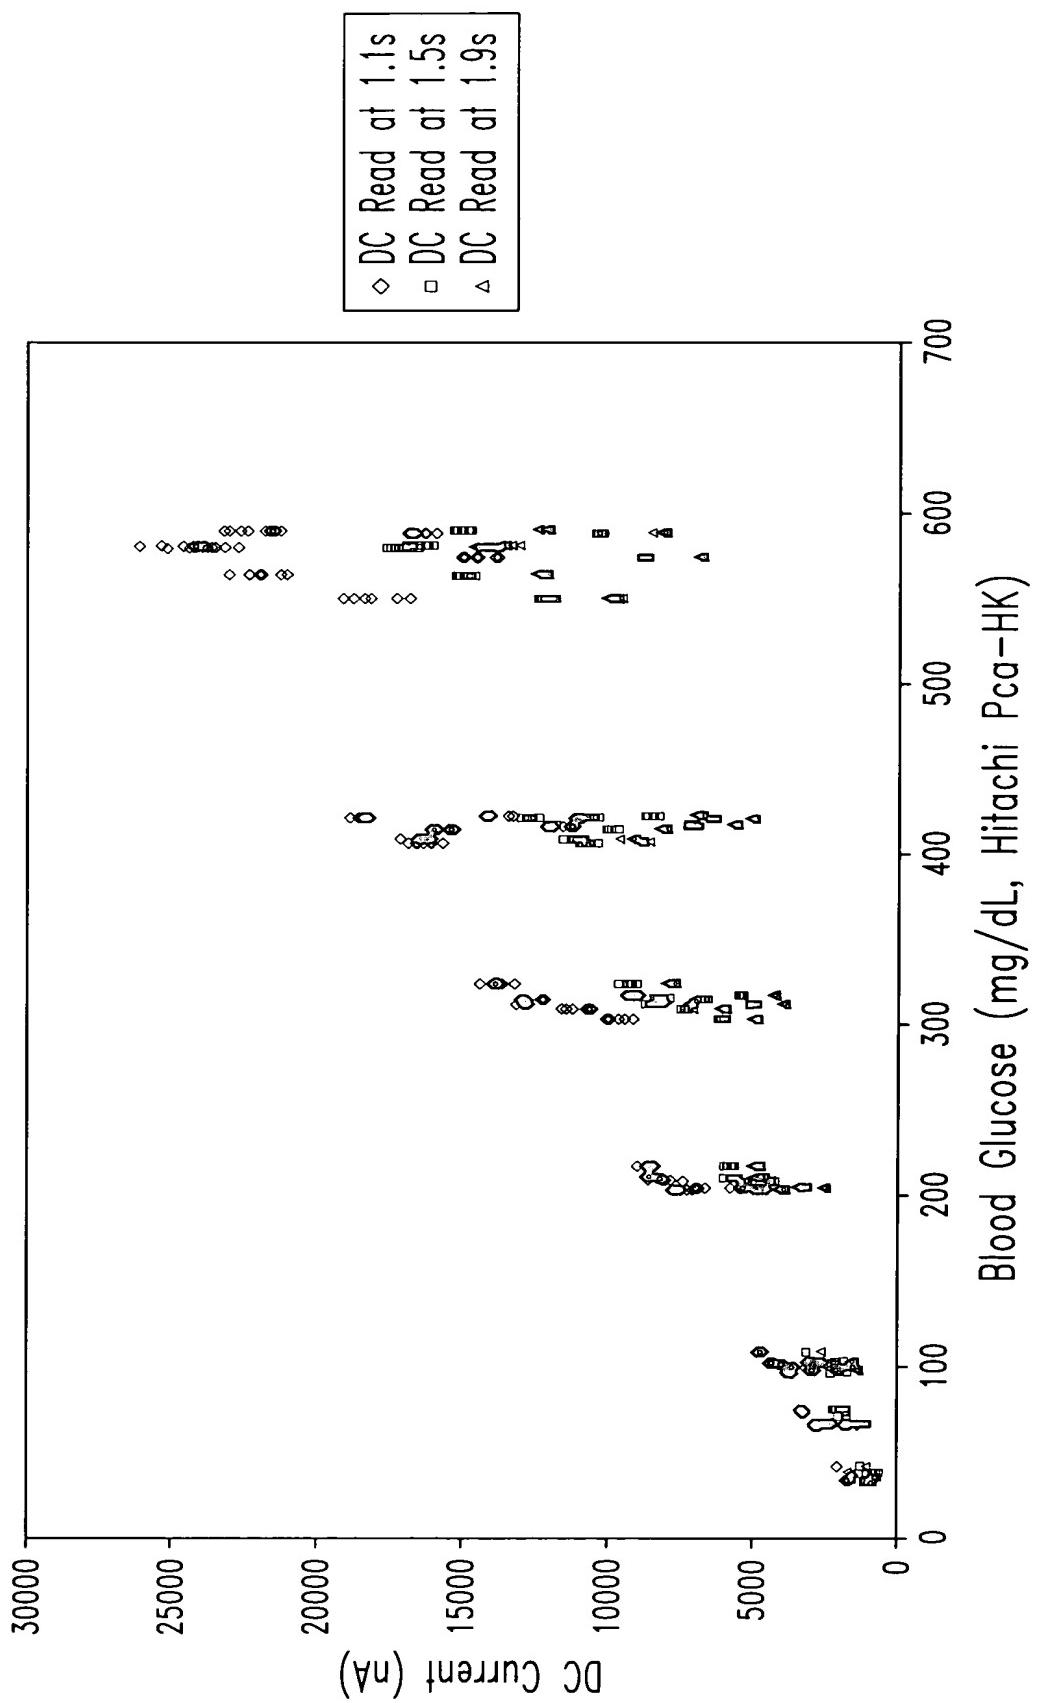


Fig. 27

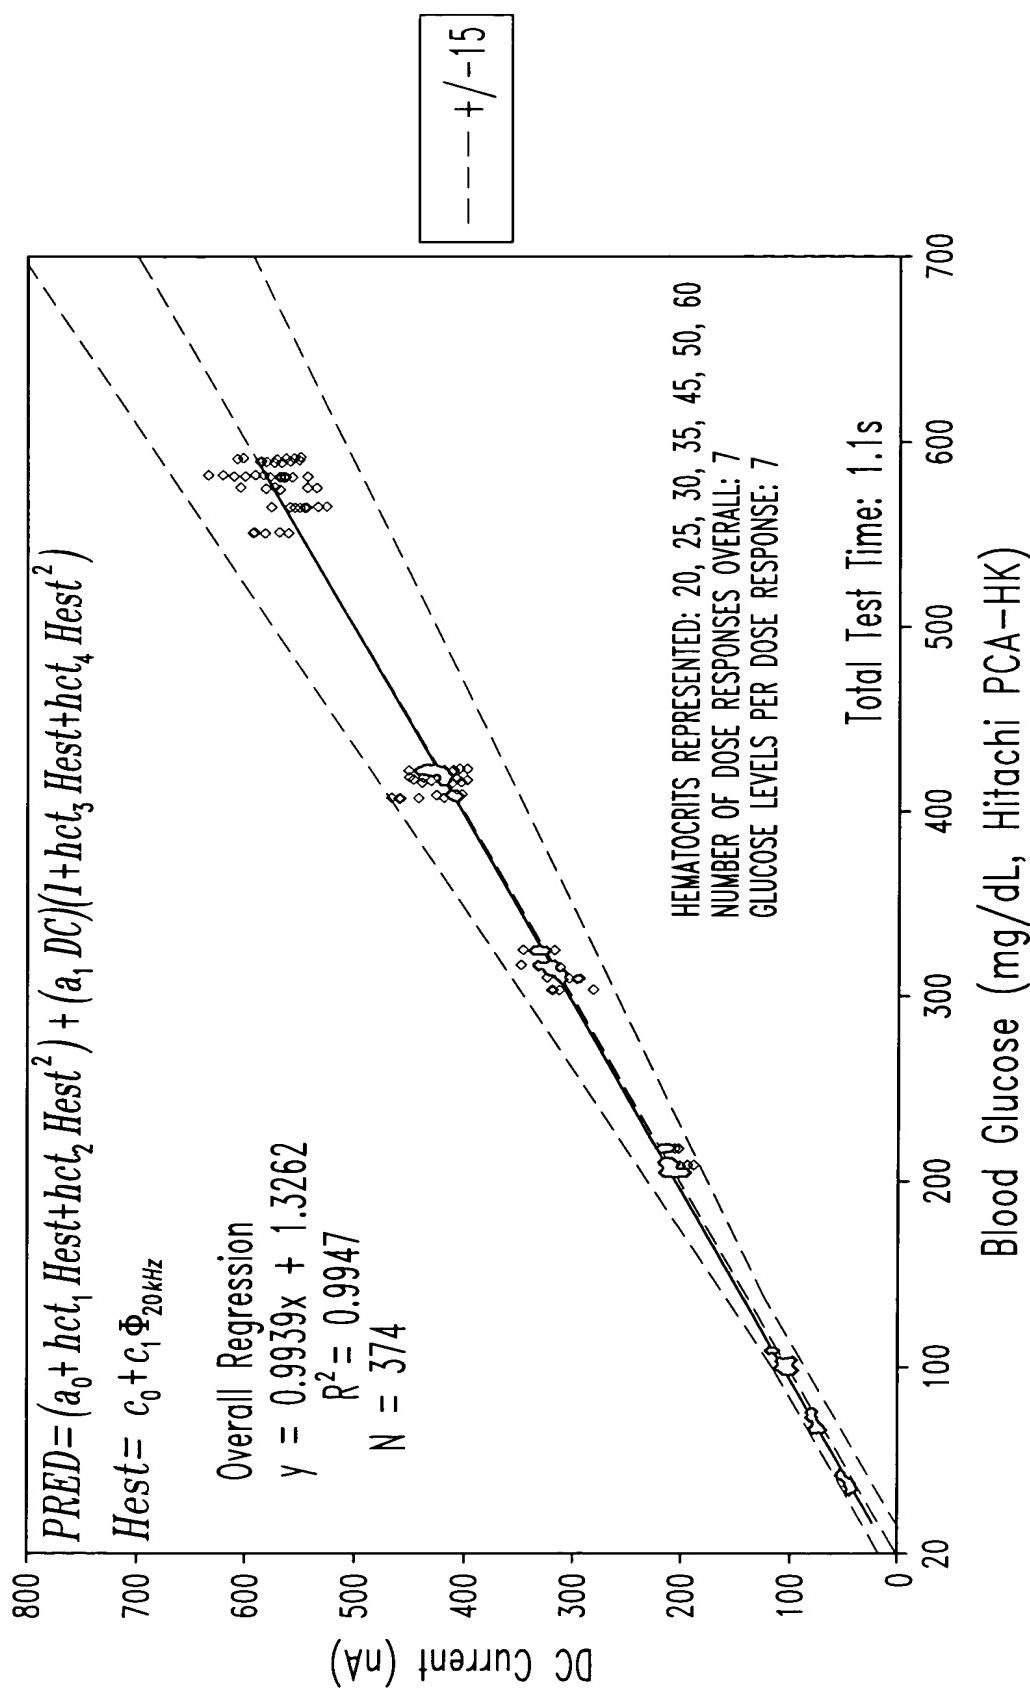


Fig. 28

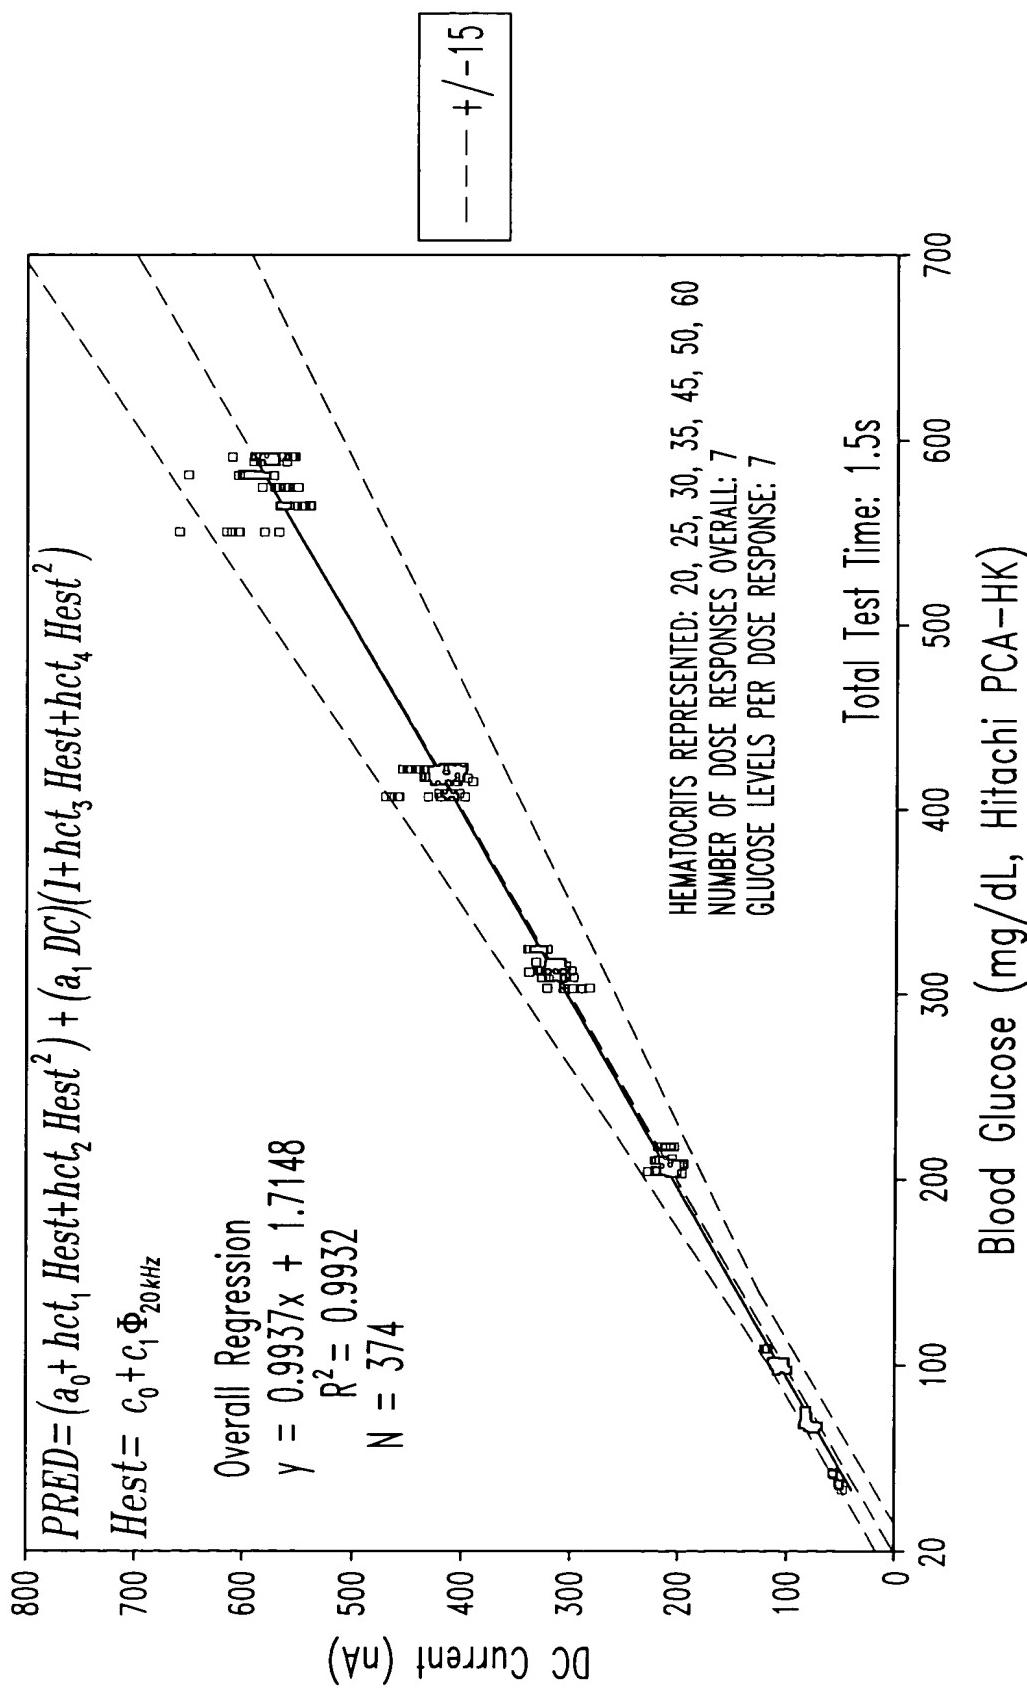


Fig. 29

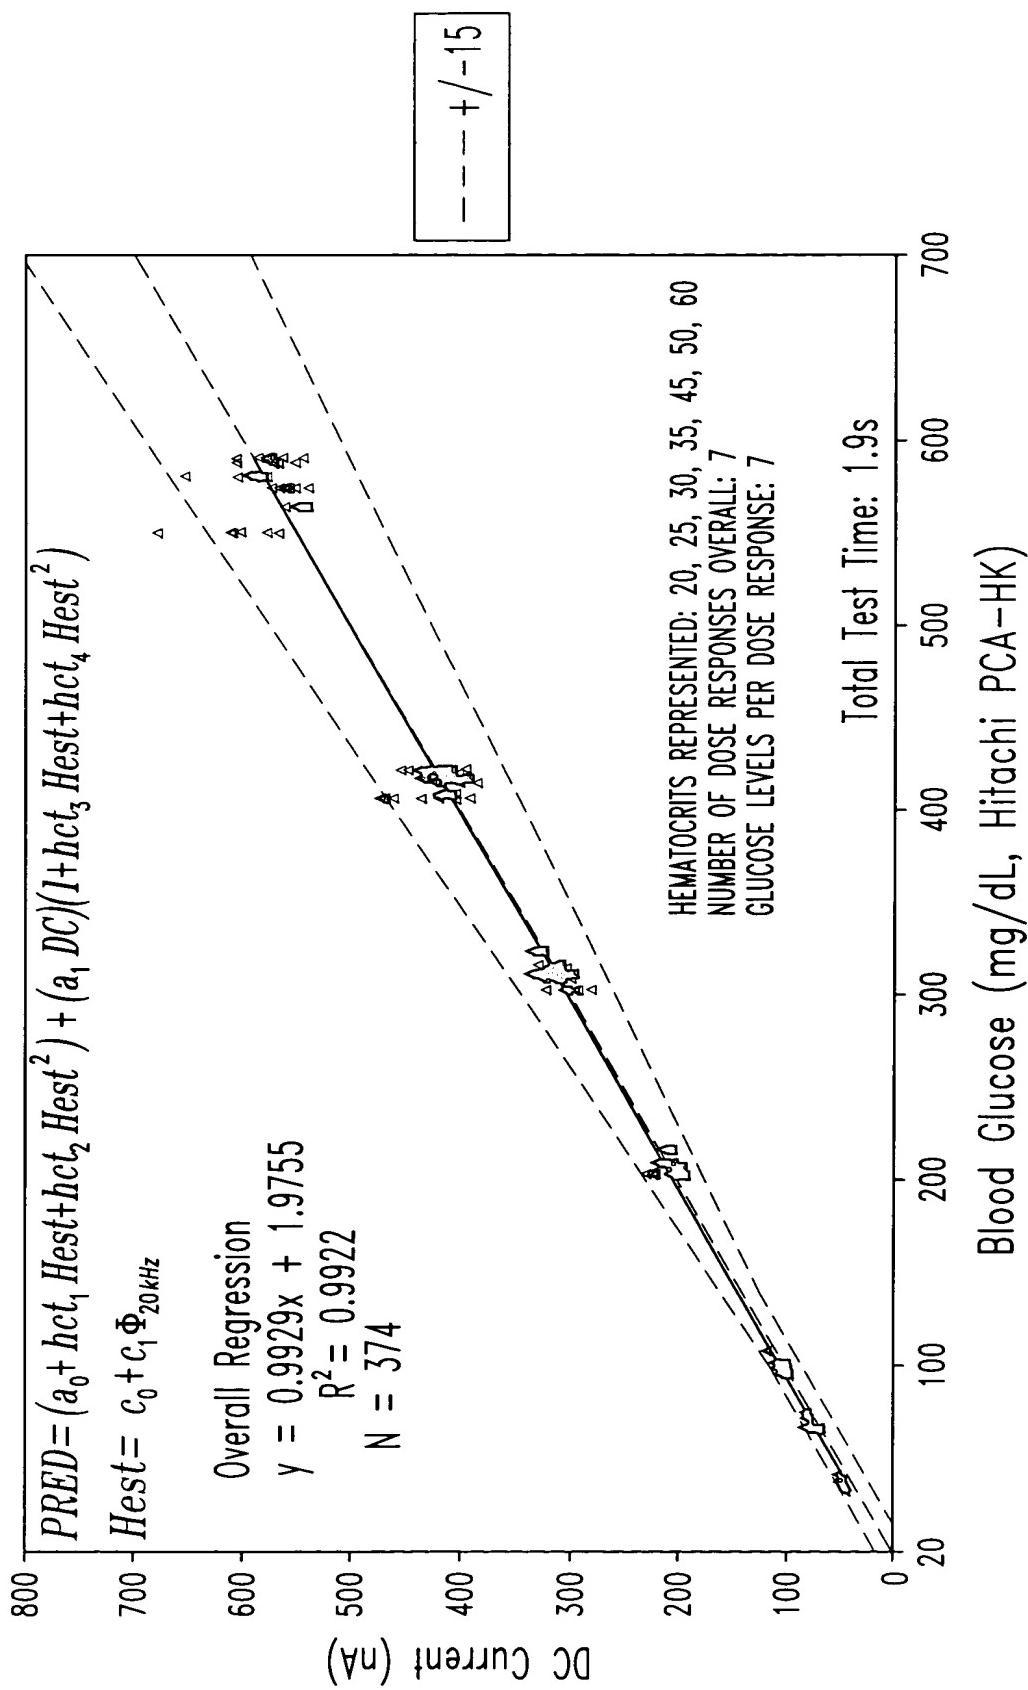


Fig. 30

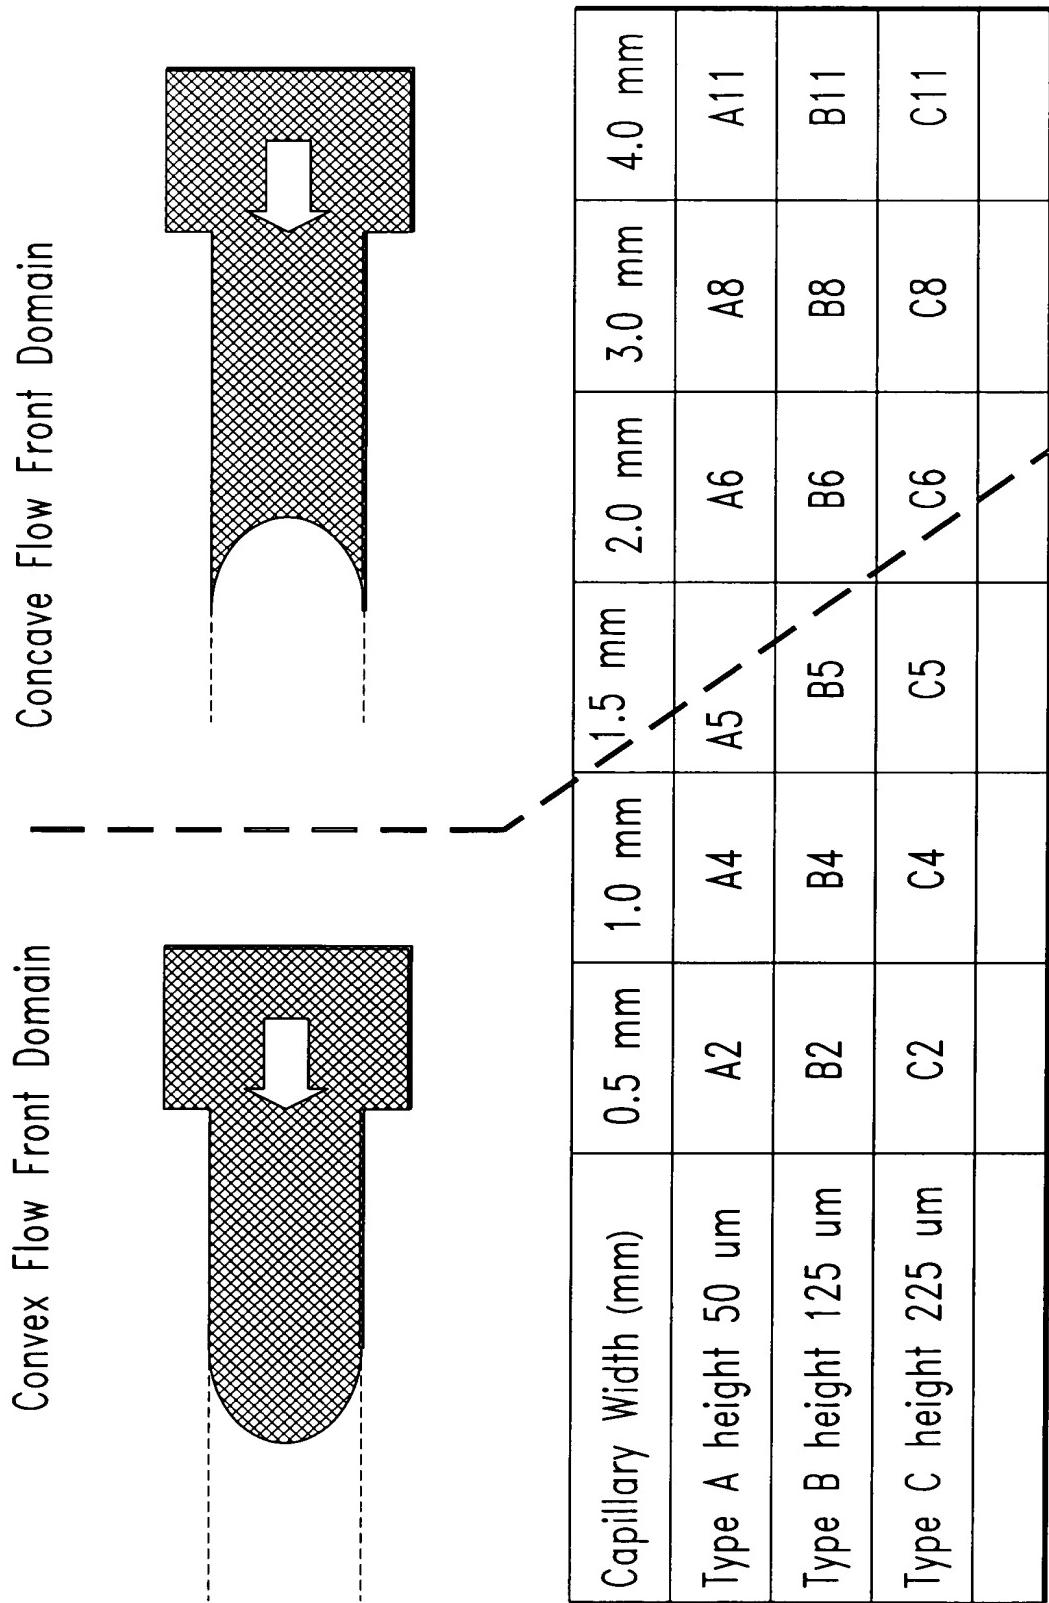


Fig. 31

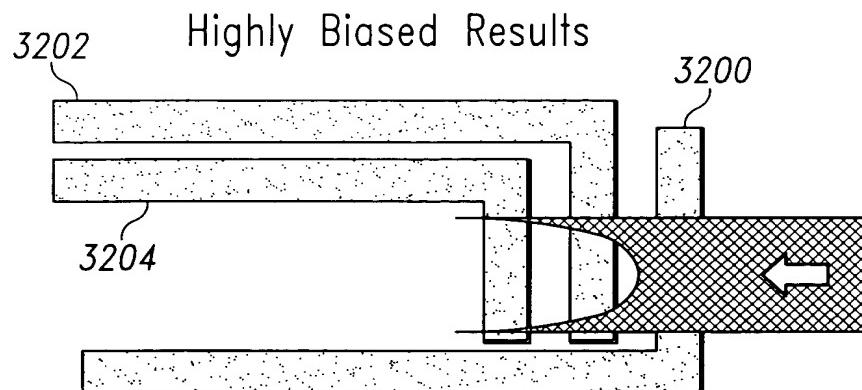


Fig. 32A

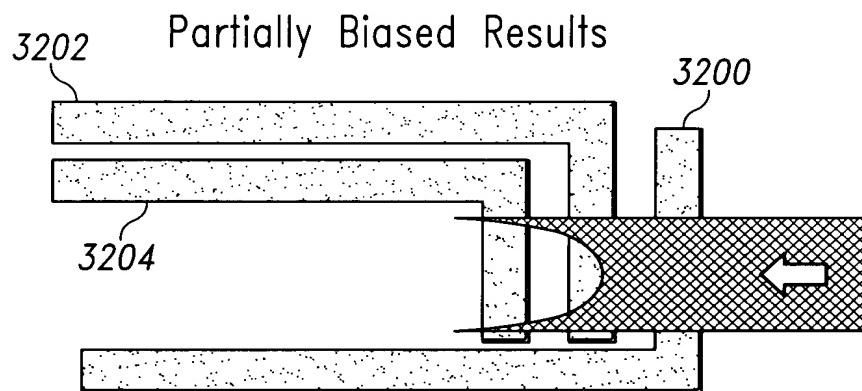


Fig. 32B

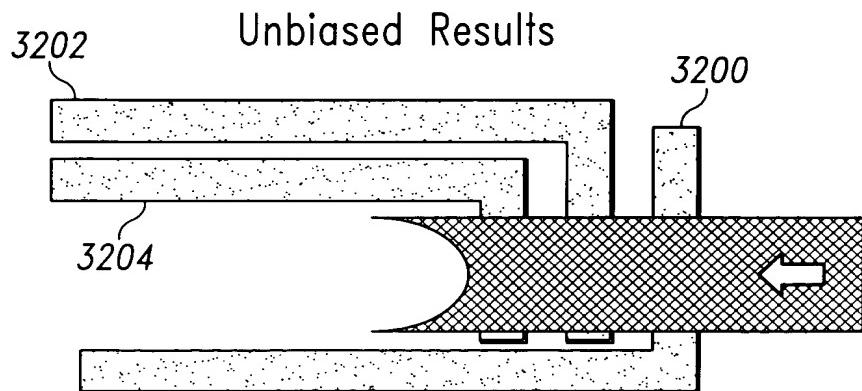


Fig. 32C

Serial No. Not Yet Assigned
Inventors: David W. Burke et al.
System and Method for Analyte Measurement
Employing Maximum Dosing Time Delay
Atty Docket: 7404-558

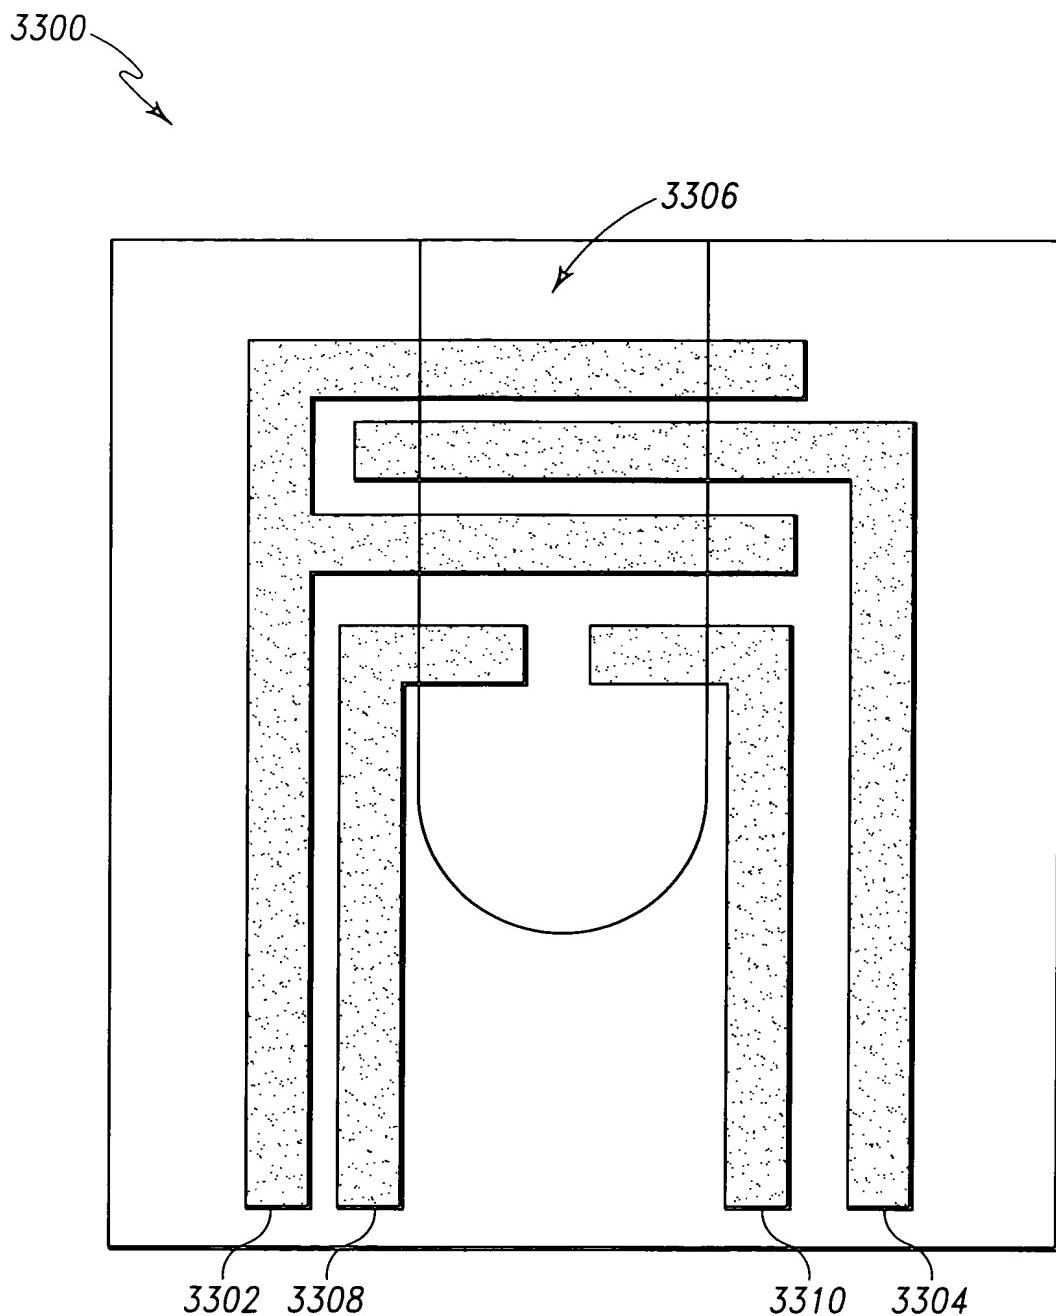


Fig. 33

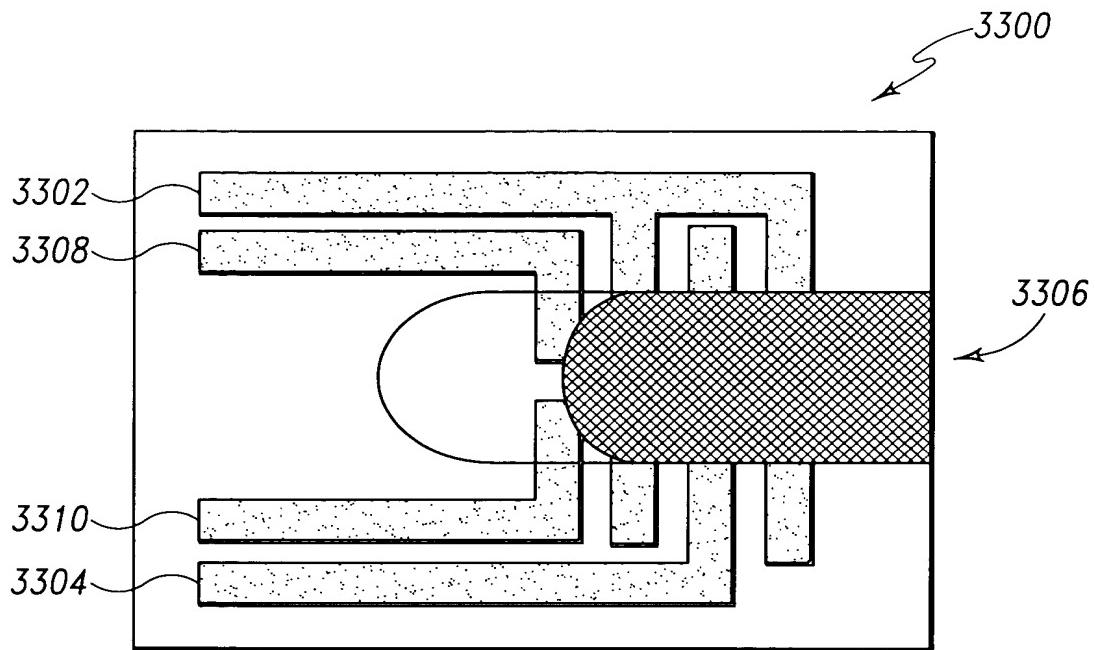


Fig. 34A

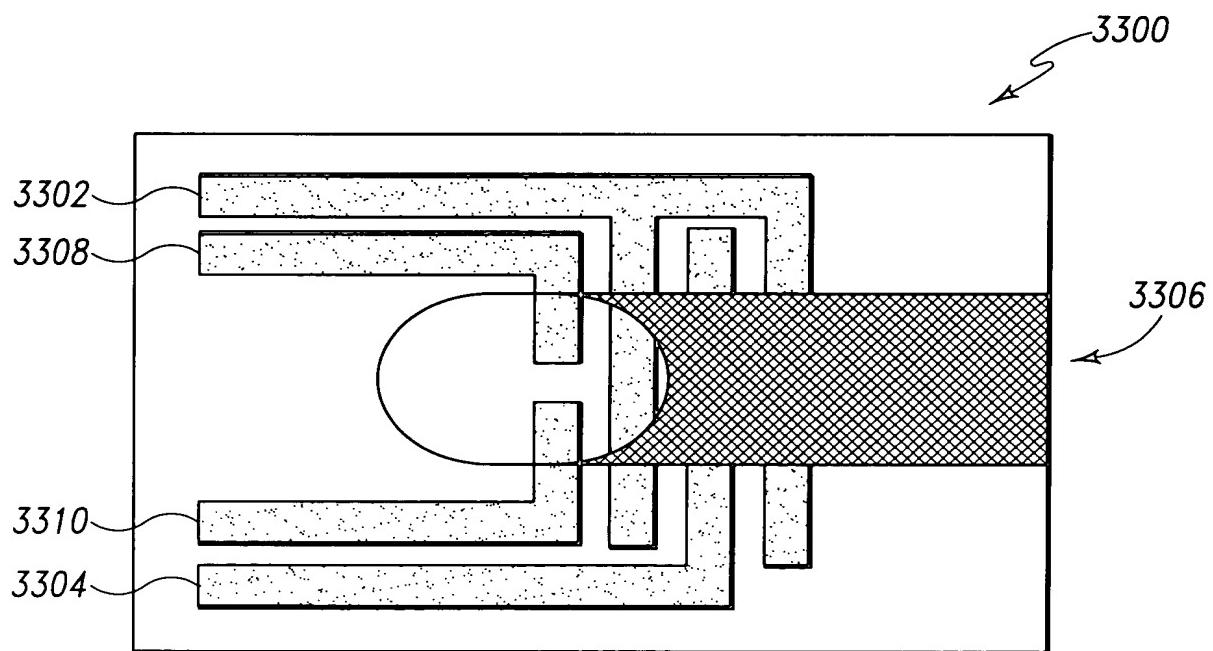


Fig. 34B

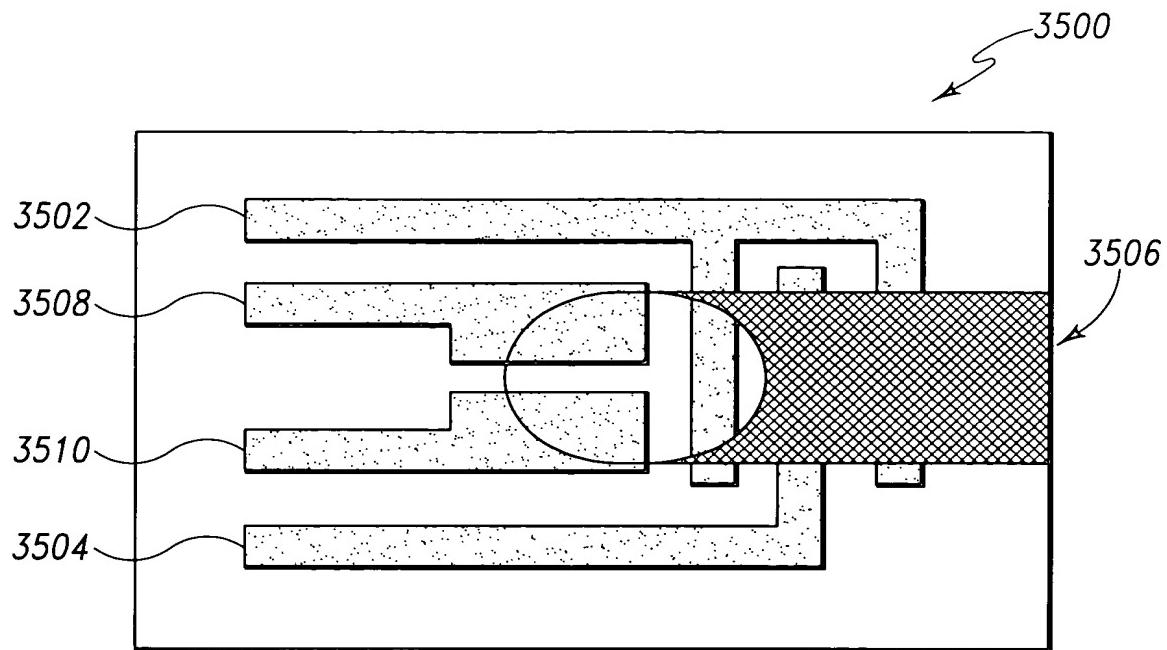


Fig. 35A

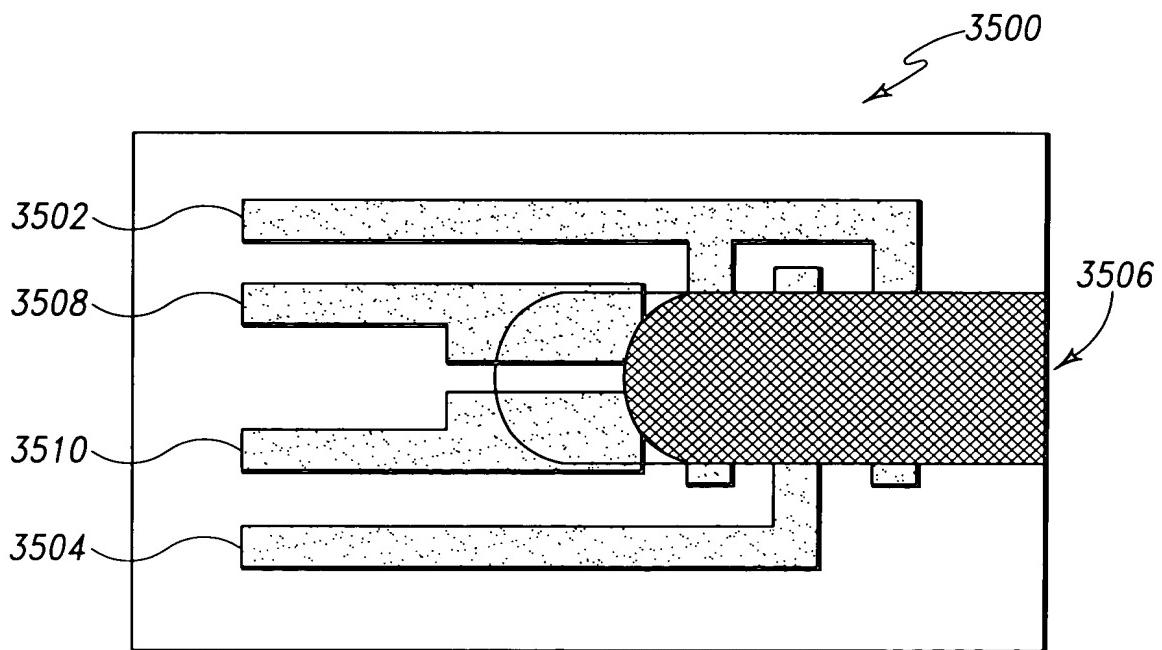


Fig. 35B

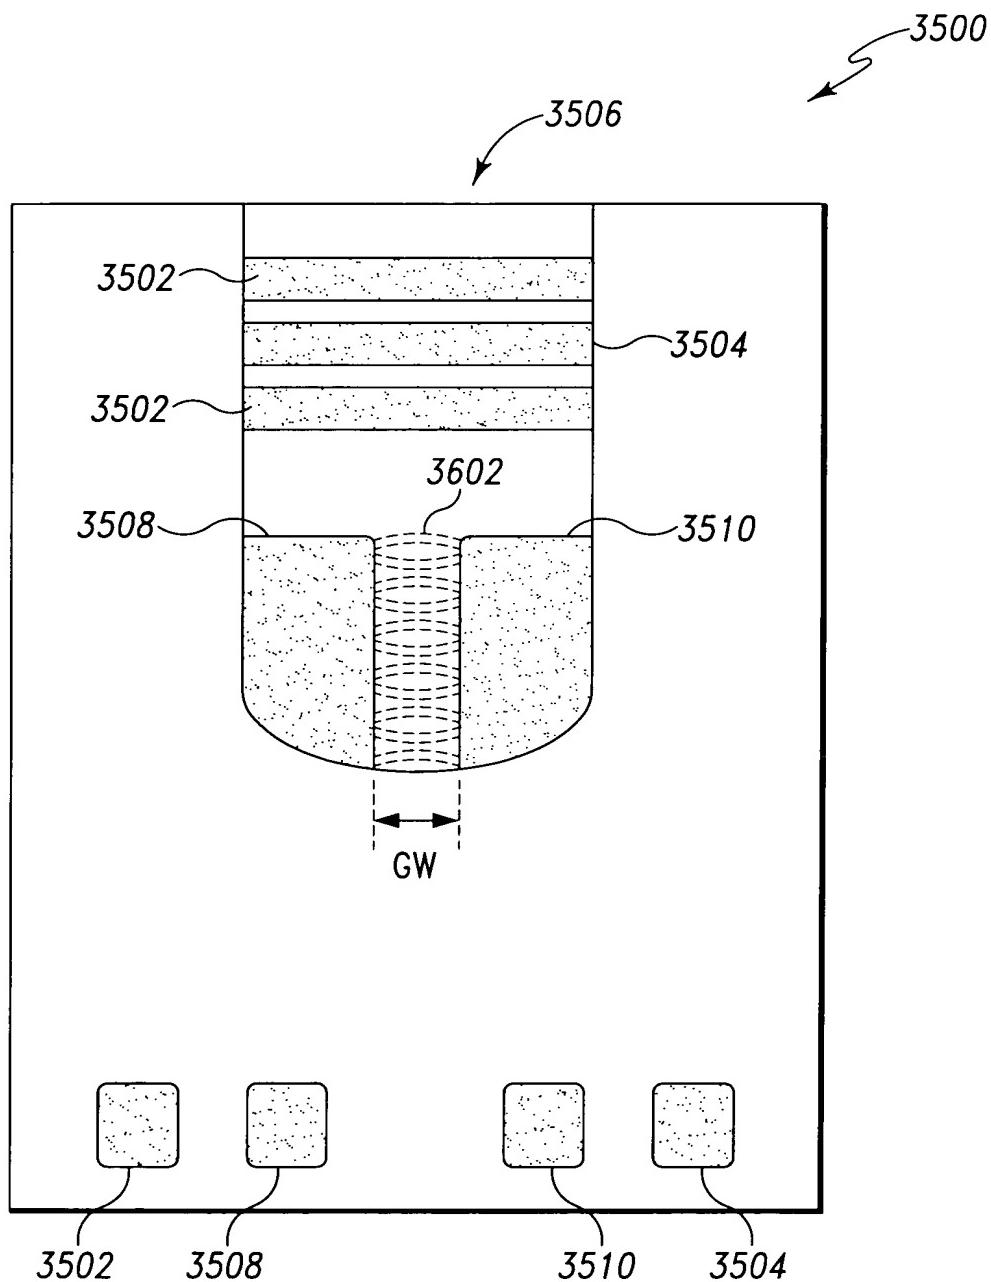


Fig. 36